

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
 Data File : VU026781.D
 Acq On : 15 Sep 2018 16:41
 Operator : MD/SY
 Sample : J4920-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KY9

Quant Time: Sep 17 06:35:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Sep 17 05:13:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	134961	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	113691	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	47921	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	47543	4.90	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.00%
7) Chloroethane-d5	1.68	69	39983	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.00%
11) 1,1-Dichloroethene-d2	2.27	63	66810	3.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.20%
20) 2-Butanone-d5	4.20	46	101154	44.71	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.42%
24) Chloroform-d	4.65	84	78149	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.31	65	42878	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.34	84	165141	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
36) 1,2-Dichloropropane-d6	6.33	67	52469	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.57	98	129219	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	7.85	79	15952	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
46) 2-Hexanone-d5	8.32	63	64890	43.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.68%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	37635	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	49028	5.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	6105	3.03 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
Data File : VU026781.D
Acq On : 15 Sep 2018 16:41
Operator : MD/SY
Sample : J4920-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KY9

Quant Time: Sep 17 06:35:48 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Sep 17 05:13:11 2018
Response via : Initial Calibration

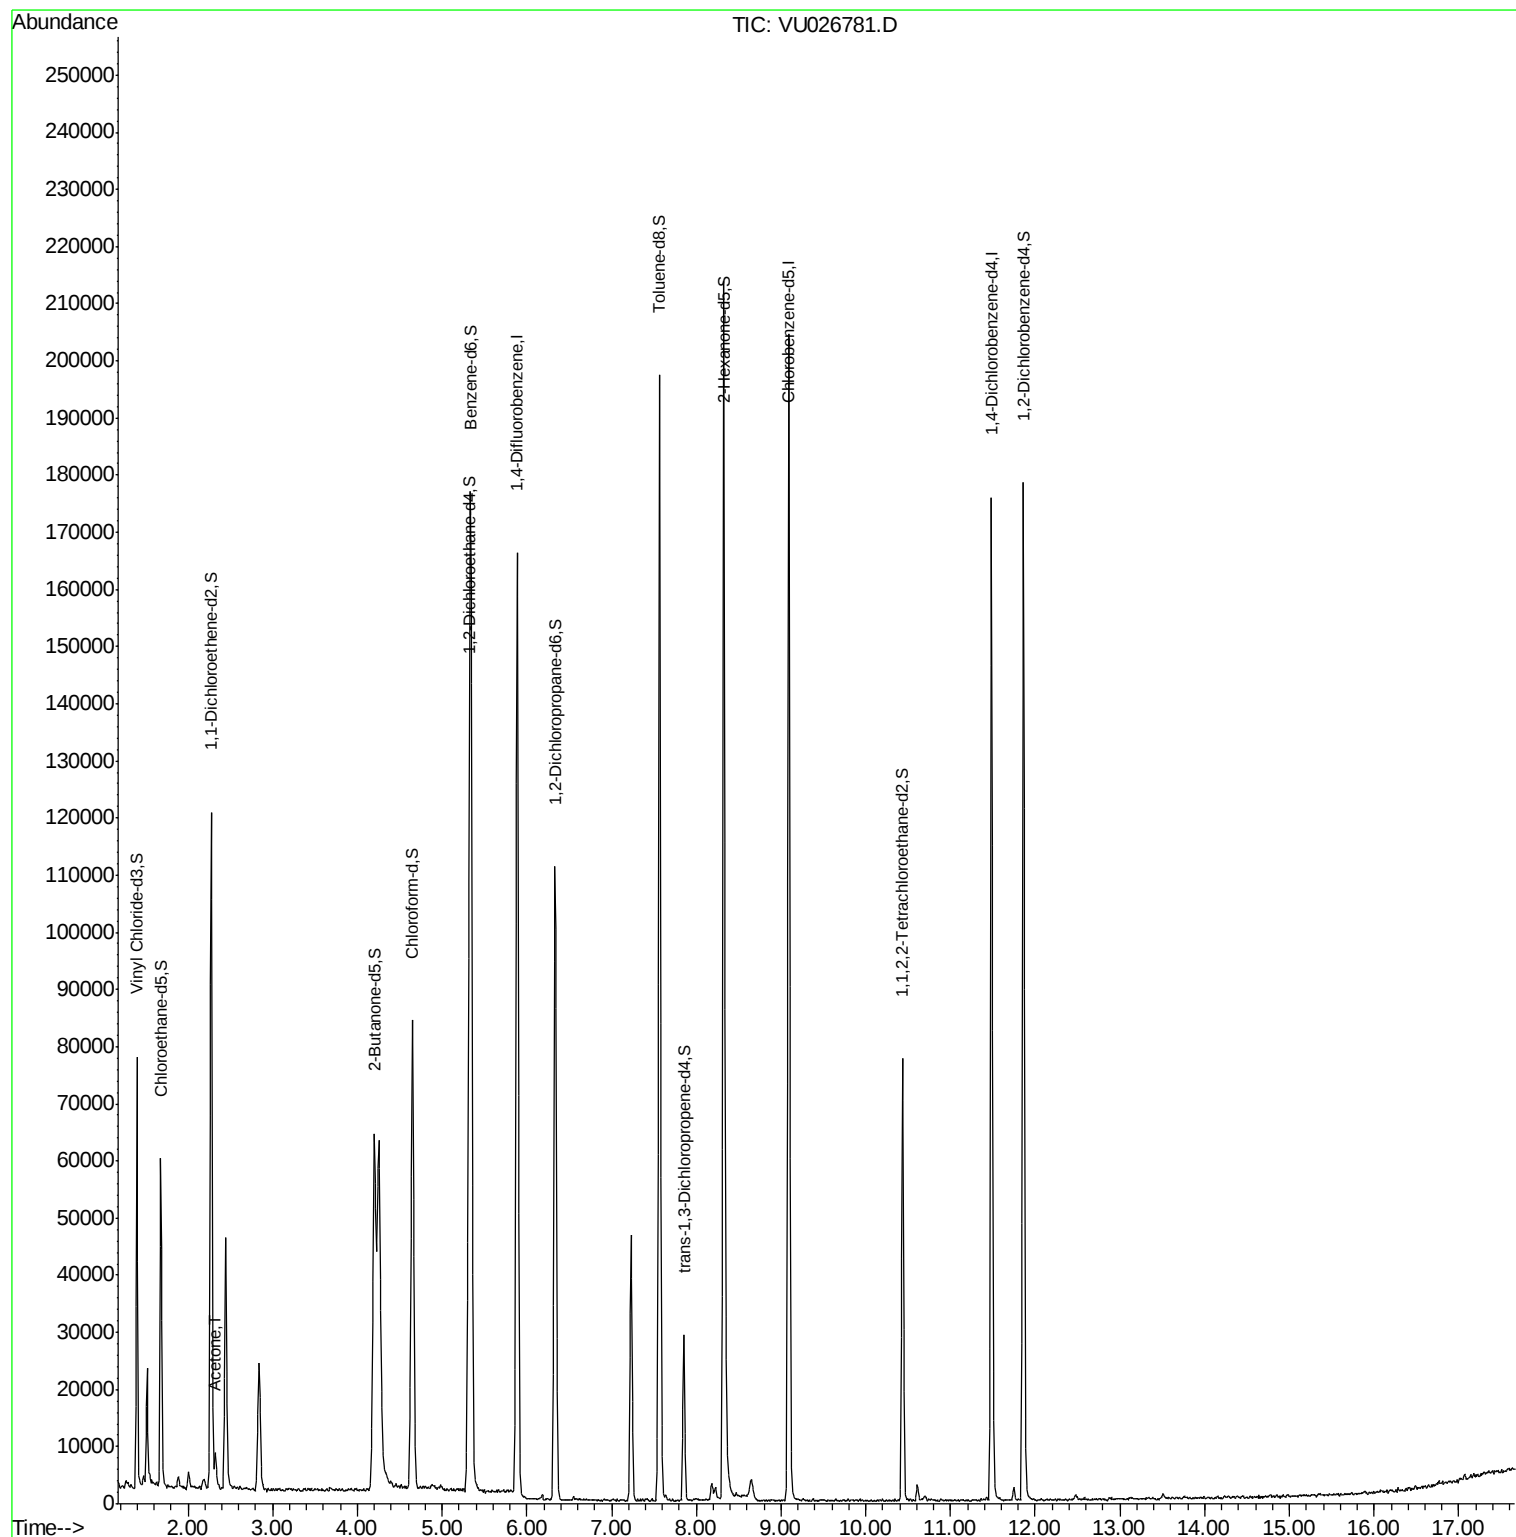

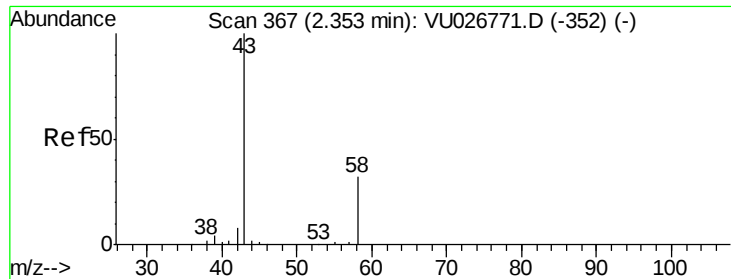

#13

Acetone

Concen: 3.03 ug/L

RT: 2.32 min Scan# 357

Delta R.T. -0.03 min

Lab File: VU026781.D

Acq: 15 Sep 2018 16:41

Instrument :
MSVOA_U
ClientSampleId :
C0KY9

Tot Ion: 43 Resp: 6105

Ion Ratio Lower Upper

43 100

58 27.0 0.0 63.0

