

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
 Data File : VU026782.D
 Acq On : 15 Sep 2018 17:07
 Operator : MD/SY
 Sample : J4920-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KZ0

Quant Time: Sep 17 06:37:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Sep 17 05:13:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	126792	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	106629	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	45078	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	46729	5.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.60%
7) Chloroethane-d5	1.68	69	38223	5.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.80%
11) 1,1-Dichloroethene-d2	2.27	63	64927	3.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.80%
20) 2-Butanone-d5	4.20	46	101932	47.96	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.92%
24) Chloroform-d	4.65	84	76616	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
26) 1,2-Dichloroethane-d4	5.31	65	41915	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
32) Benzene-d6	5.34	84	160738	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.80%
36) 1,2-Dichloropropane-d6	6.33	67	50769	5.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.80%
41) Toluene-d8	7.57	98	125044	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.85	79	15827	4.45	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.00%
46) 2-Hexanone-d5	8.32	63	64632	46.03	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.06%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	37515	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	46075	5.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	7847	4.15 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
Data File : VU026782.D
Acq On : 15 Sep 2018 17:07
Operator : MD/SY
Sample : J4920-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KZ0

Quant Time: Sep 17 06:37:38 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Sep 17 05:13:11 2018
Response via : Initial Calibration

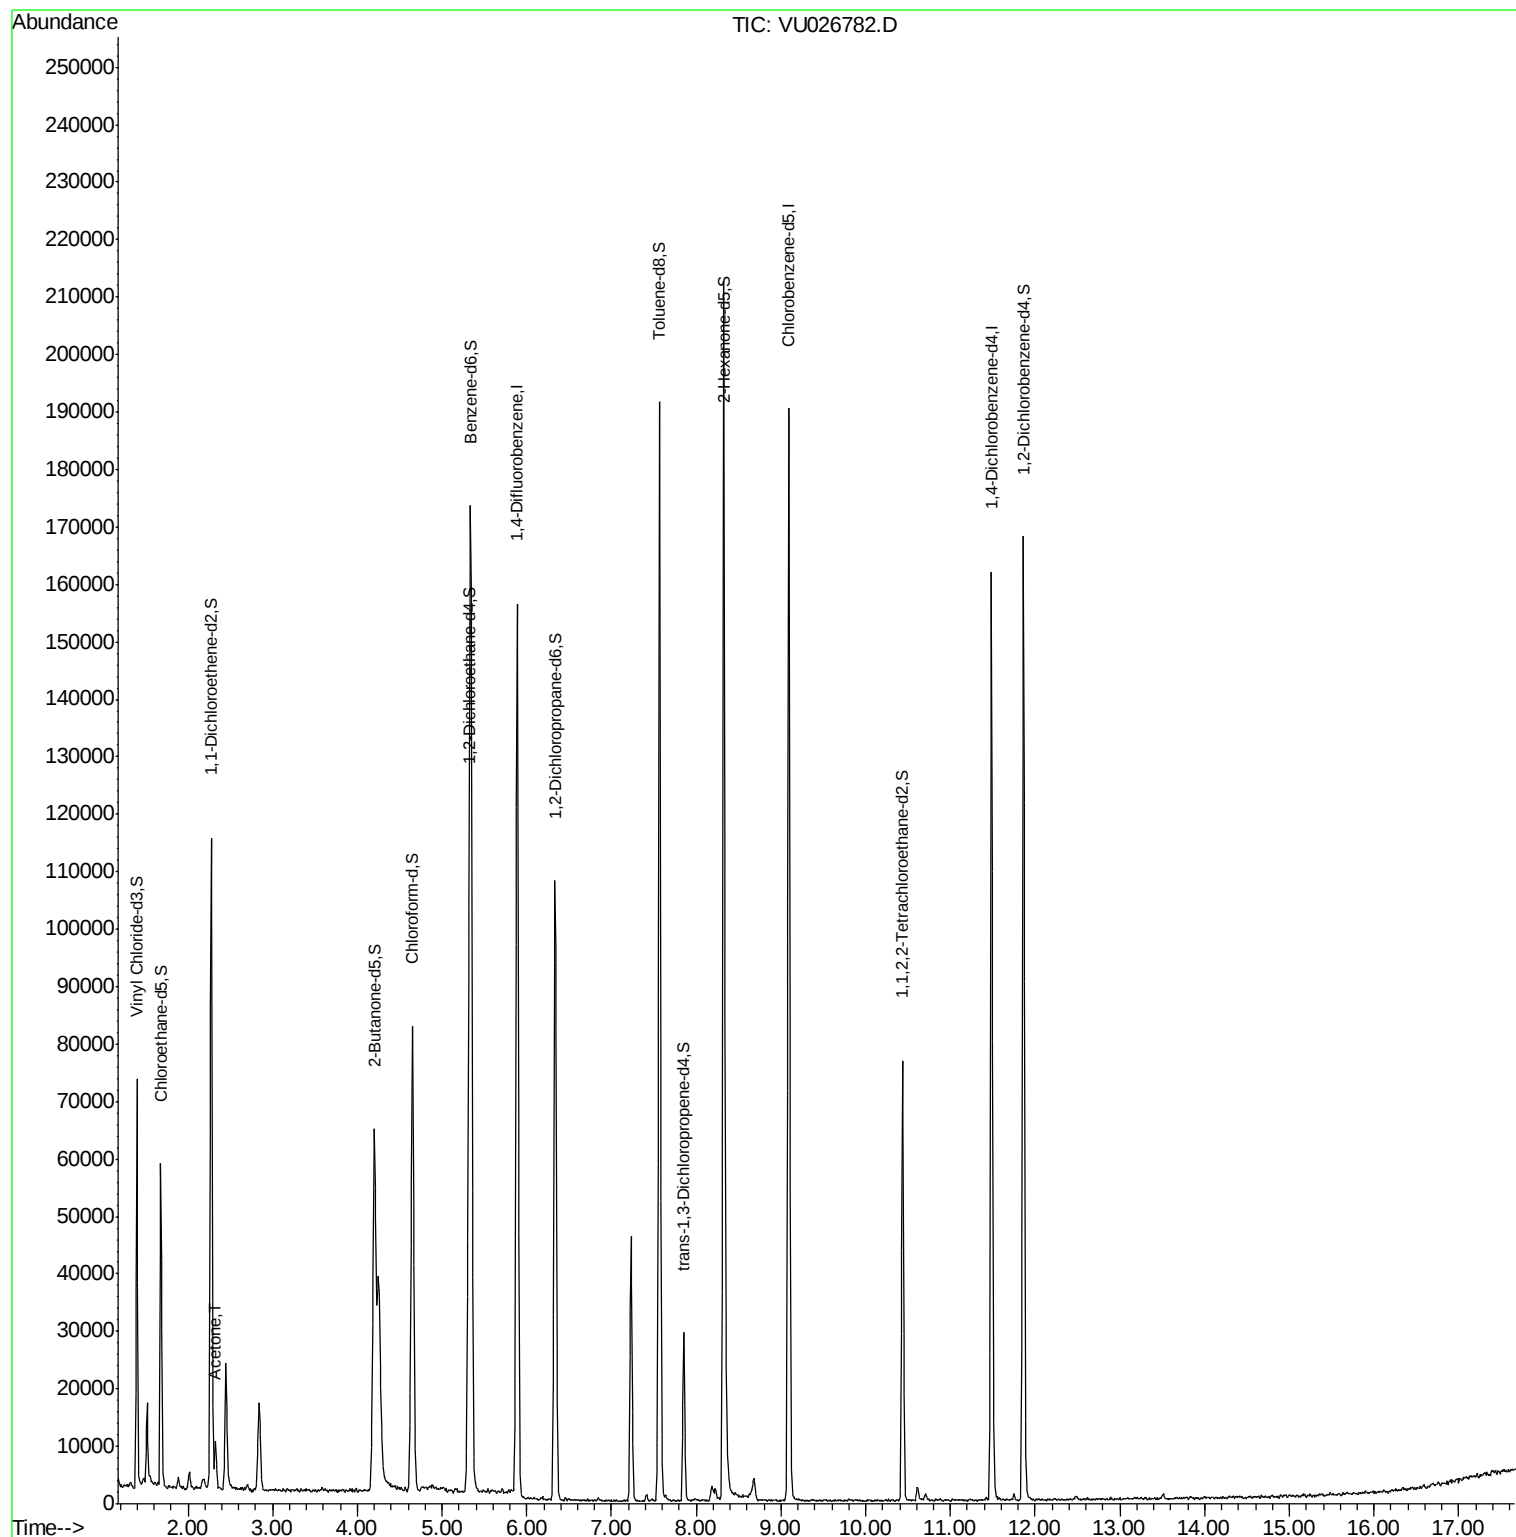

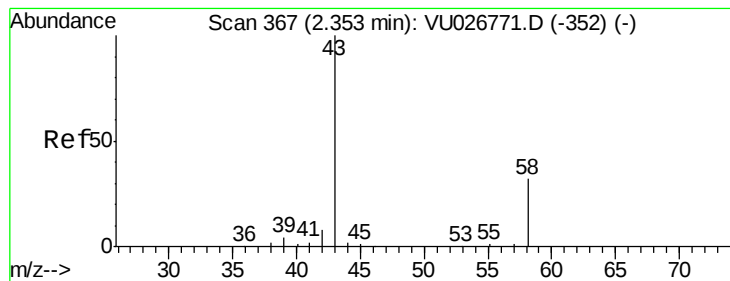

#13
 Acetone
 Concen: 4.15 ug/L
 RT: 2.32 min Scan# 358
 Delta R.T. -0.03 min
 Lab File: VU026782.D
 Acq: 15 Sep 2018 17:07

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KZ0

Tot Ion: 43 Resp: 7847
 Ion Ratio Lower Upper
 43 100
 58 29.6 0.0 63.0

