

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
 Data File : VU026791.D
 Acq On : 15 Sep 2018 21:02
 Operator : MD/SY
 Sample : J4920-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KZ9

Quant Time: Sep 17 09:49:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Sep 17 05:13:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	121121	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	100307	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	39753	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	46258	5.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.40%
7) Chloroethane-d5	1.68	69	38162	5.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.40%
11) 1,1-Dichloroethene-d2	2.27	63	64293	3.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.40%
20) 2-Butanone-d5	4.20	46	102679	50.57	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.14%
24) Chloroform-d	4.65	84	78604	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
26) 1,2-Dichloroethane-d4	5.31	65	41969	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.60%
32) Benzene-d6	5.34	84	163006	5.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.20%
36) 1,2-Dichloropropane-d6	6.33	67	50667	5.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.40%
41) Toluene-d8	7.57	98	124286	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
43) trans-1,3-Dichloropropene-	7.85	79	14847	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.32	63	63660	48.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.38%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	37842	5.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	45116	6.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.20%#


Target Compounds					Ovalue
13) Acetone	2.32	43	5666	3.14 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
Data File : VU026791.D
Acq On : 15 Sep 2018 21:02
Operator : MD/SY
Sample : J4920-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KZ9

Quant Time: Sep 17 09:49:47 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Sep 17 05:13:11 2018
Response via : Initial Calibration

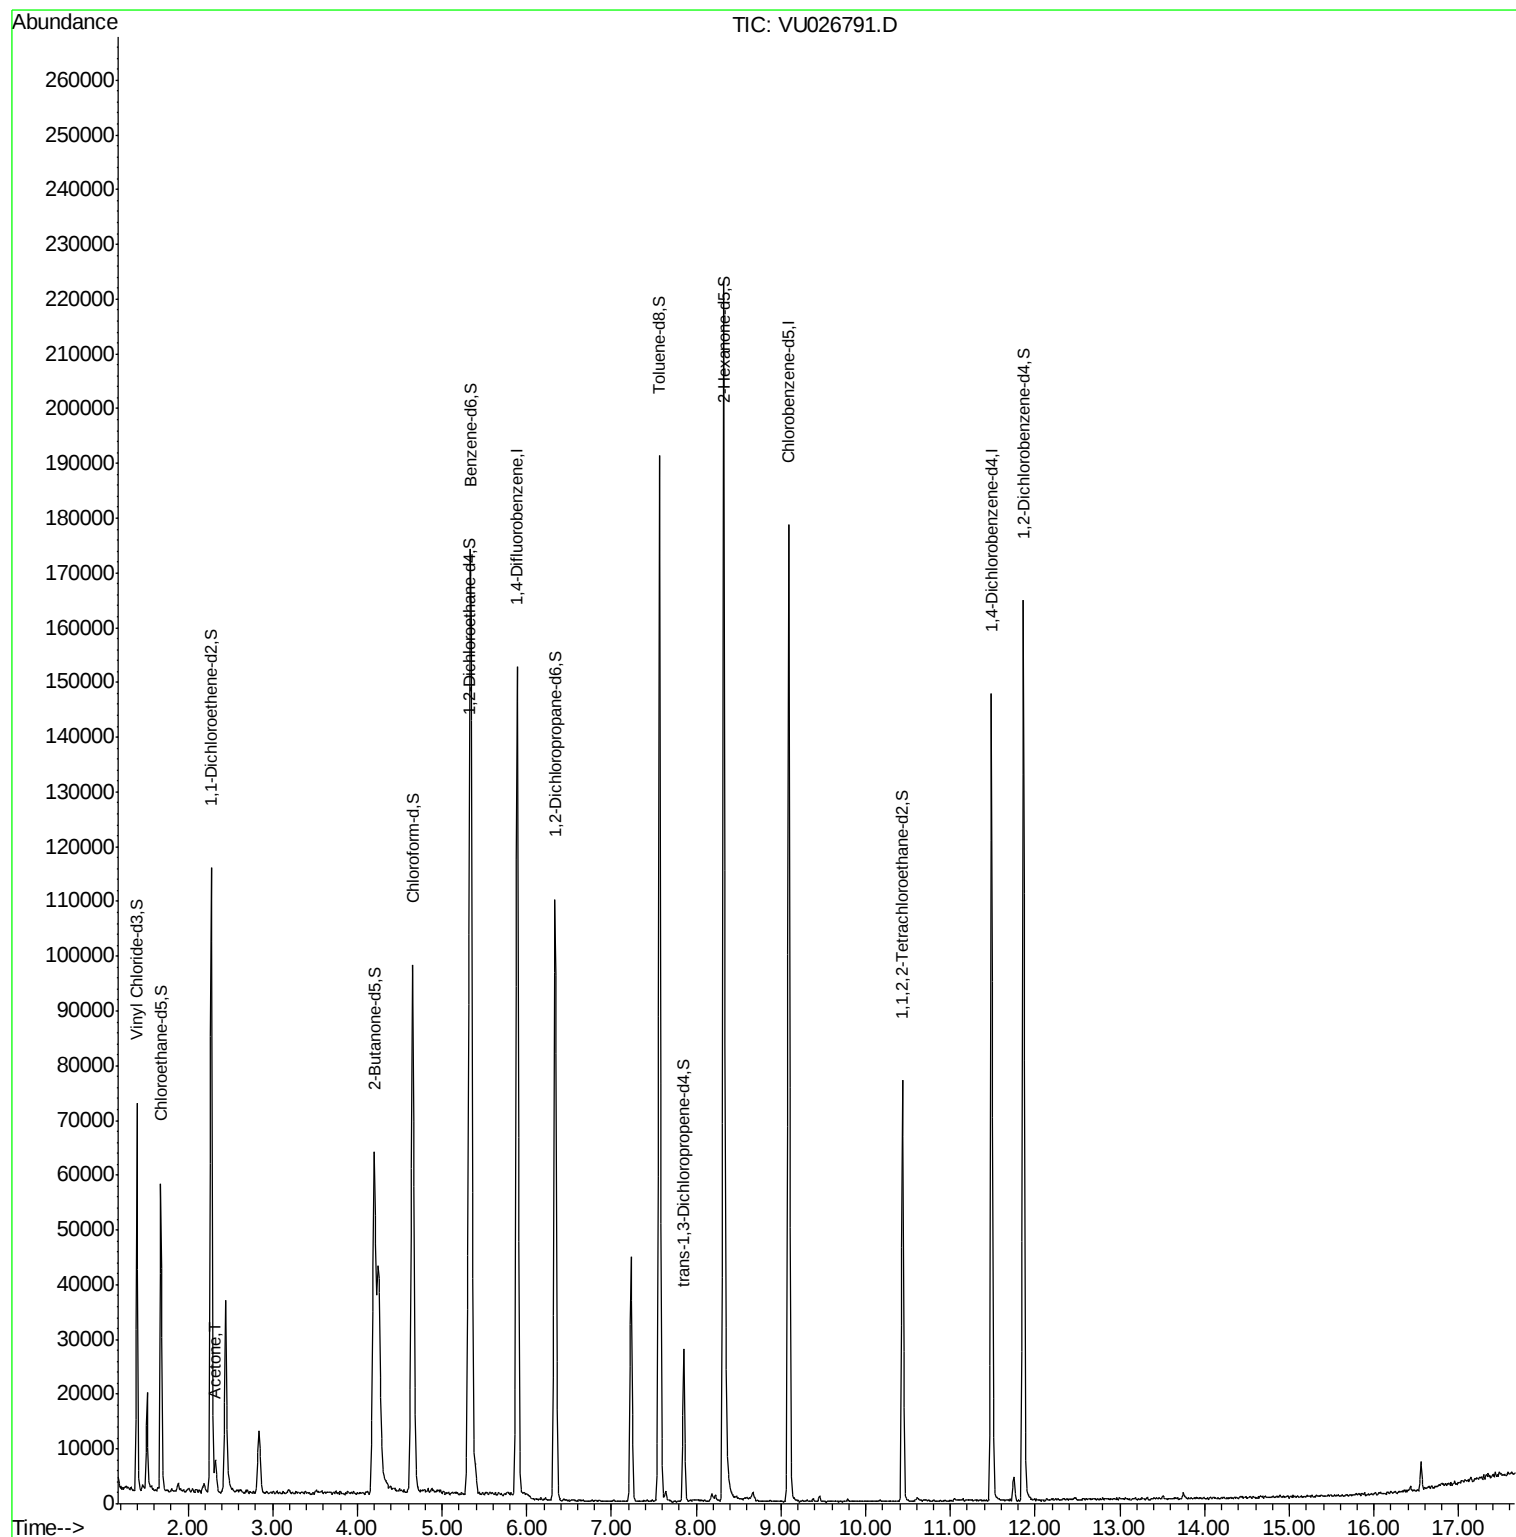

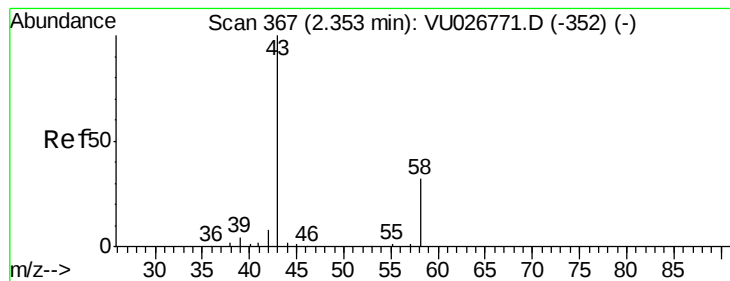

#13
 Acetone
 Concen: 3.14 ug/L
 RT: 2.32 min Scan# 357
 Delta R.T. -0.03 min
 Lab File: VU026791.D
 Acq: 15 Sep 2018 21:02

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KZ9

Tot Ion: 43 Resp: 5666
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 63.0

