

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
 Data File : VU026788.D
 Acq On : 15 Sep 2018 19:44
 Operator : MD/SY
 Sample : J4920-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KZ6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	62	70	87	rBV	74192	75945	17.16%	2.188%
2	1.517	100	107	120	rBV	18403	20891	4.72%	0.602%
3	1.681	150	158	173	rVB	54248	67921	15.34%	1.957%
4	2.276	331	343	354	rBV	111470	169288	38.25%	4.877%
5	2.324	354	358	368	rVB4	3032	4581	1.03%	0.132%
6	2.447	386	396	402	rBV	26624	46358	10.47%	1.336%
7	2.697	467	474	488	rBV2	5439	9175	2.07%	0.264%
8	2.839	506	518	535	rVB2	21118	45707	10.33%	1.317%
9	2.939	541	549	562	rVB3	2735	5063	1.14%	0.146%
10	4.199	921	941	951	rBV	62080	165835	37.47%	4.778%
11	4.649	1065	1081	1099	rBV	77635	179891	40.64%	5.183%
12	5.337	1273	1295	1315	rBV2	168514	442628	100.00%	12.752%
13	5.887	1451	1466	1481	rBV	151344	285784	64.57%	8.233%
14	6.334	1590	1605	1626	rBV	104829	207113	46.79%	5.967%
15	7.231	1872	1884	1898	rBV	41674	72482	16.38%	2.088%
16	7.565	1975	1988	2006	rBV	182559	314876	71.14%	9.072%
17	7.852	2066	2077	2090	rBV	25786	42698	9.65%	1.230%
18	8.183	2169	2180	2188	rBV3	2501	4598	1.04%	0.132%
19	8.324	2211	2224	2256	rBV	201057	359734	81.27%	10.364%
20	9.093	2450	2463	2481	rBV	183083	303301	68.52%	8.738%
21	9.610	2613	2624	2634	rBV2	6353	10182	2.30%	0.293%
22	10.433	2870	2880	2897	rVB	73437	117272	26.49%	3.379%
23	11.485	3196	3207	3230	rBV	158453	251968	56.93%	7.259%
24	11.745	3281	3288	3300	rVB4	3509	5779	1.31%	0.166%
25	11.861	3310	3324	3344	rBV	163832	261968	59.18%	7.547%


Sum of corrected areas: 3471038

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091618\
Data File : VU026788.D
Acq On : 15 Sep 2018 19:44
Operator : MD/SY
Sample : J4920-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0KZ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

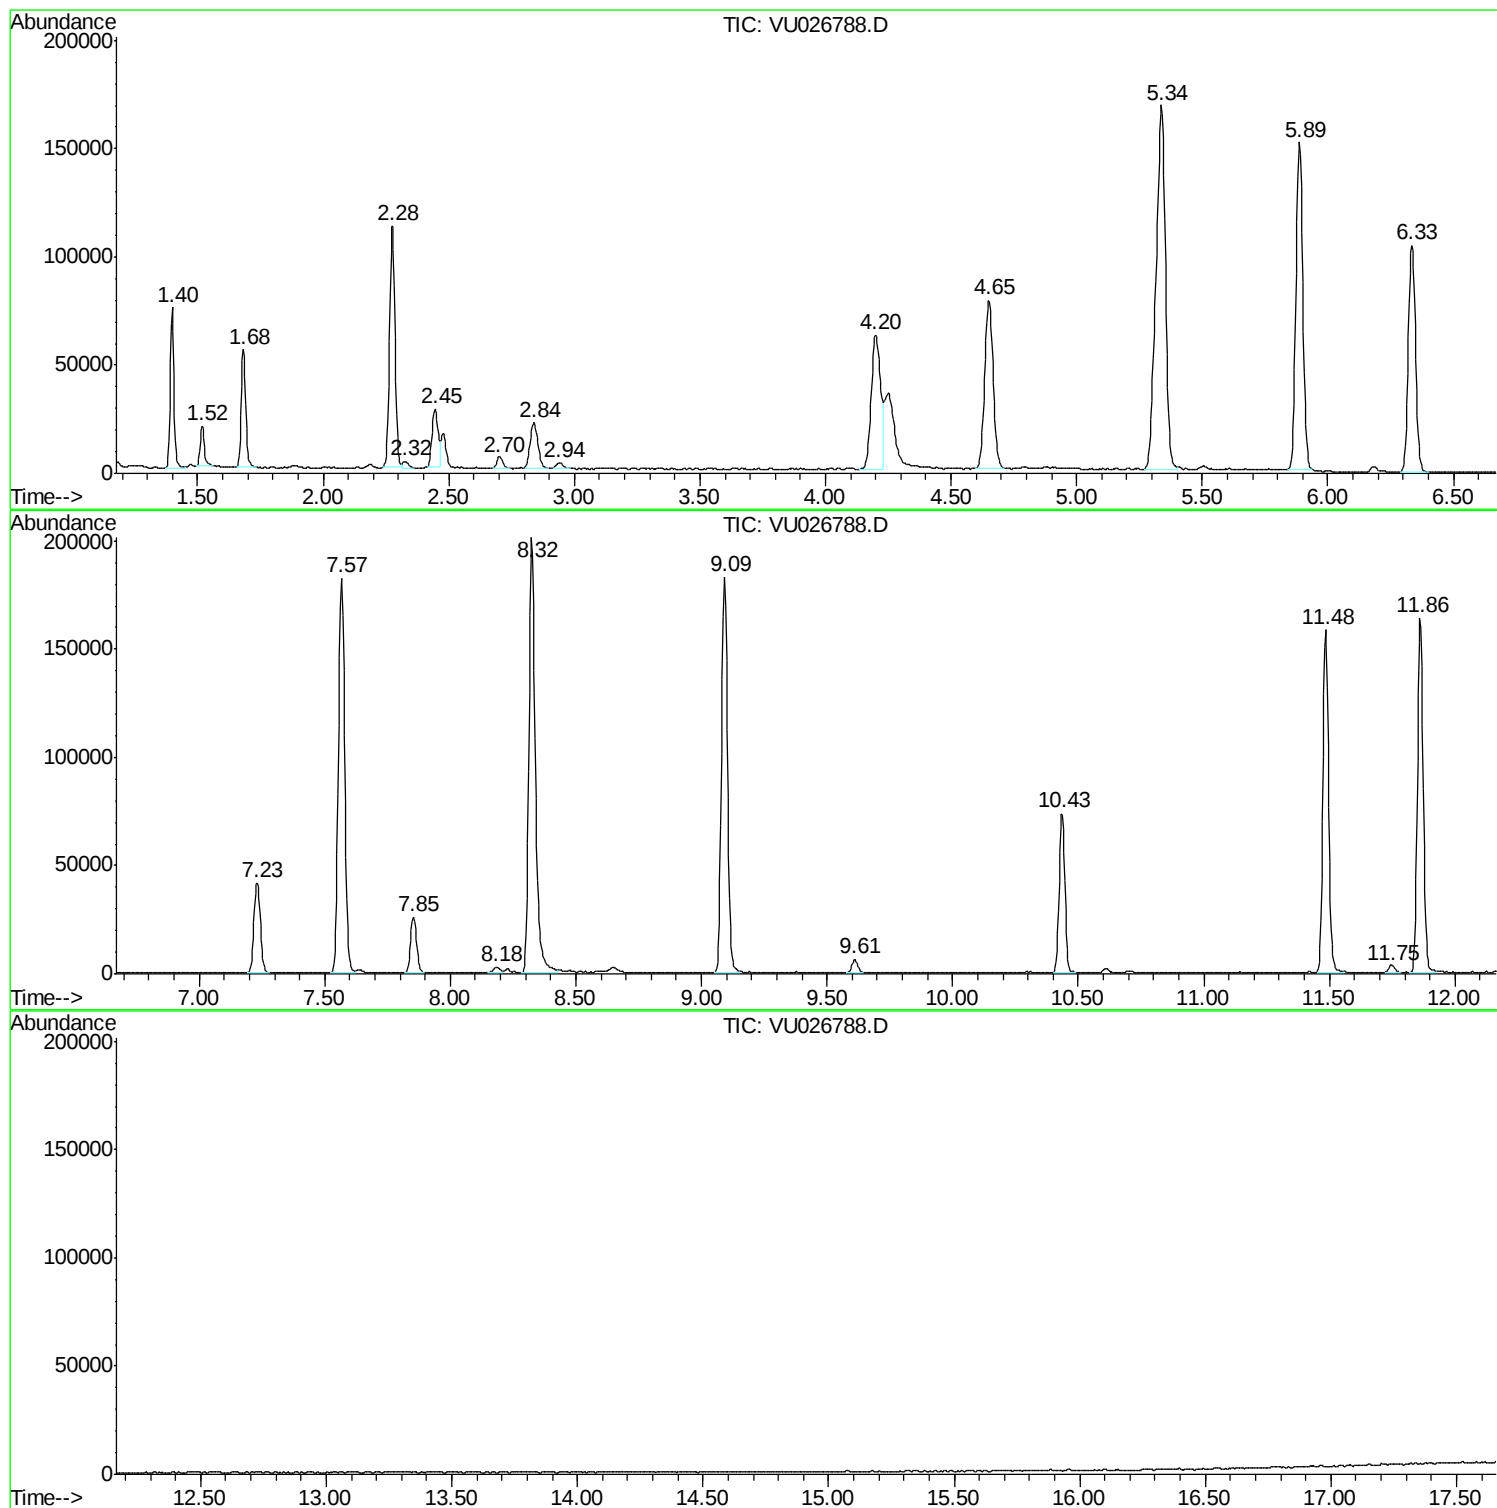

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091618\
Data File : VU026788.D
Acq On : 15 Sep 2018 19:44
Operator : MD/SY
Sample : J4920-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KZ6










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Cyclopentene, 1,4-bis(met... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.84	0.80 ug/L	45707	1,4-Difluorobenzene	5.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Cyclopentene, 1,4-bis(methoxve...	276	C13H24O6	1000156-00-3	83
2		Silane, (2-methoxvethyl)trimethyl-	132	C6H16OSi	018173-63-2	74
3		Tricvclo[5.2.2.0(2,6)]undecan-11...	352	C18H24O7	1000155-17-7	64
4		Silane, methoxyvtrimethyl-	104	C4H12OSi	001825-61-2	56
5		Silane, methoxytrimethyl-	104	C4H12OSi	001825-61-2	50

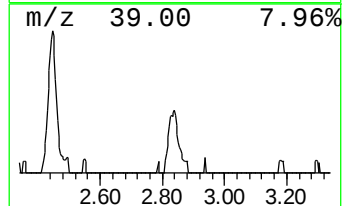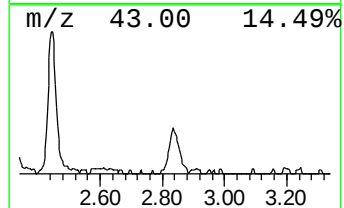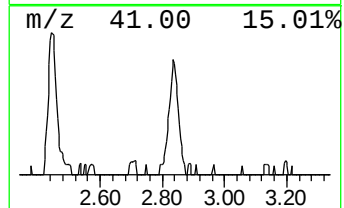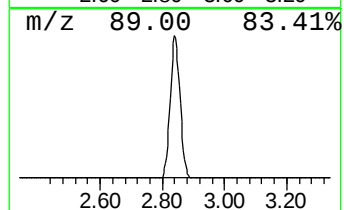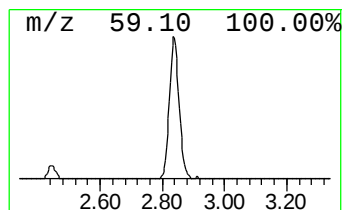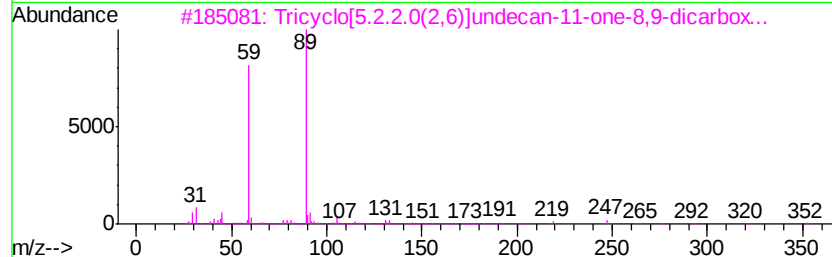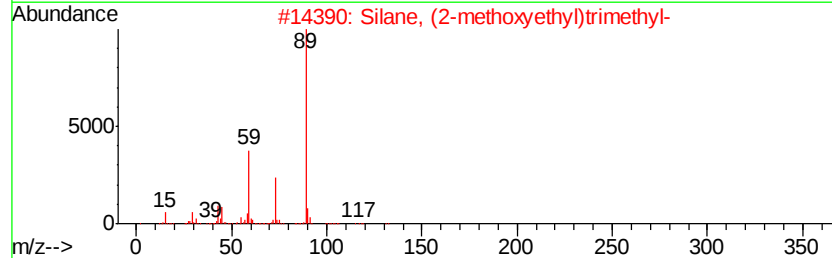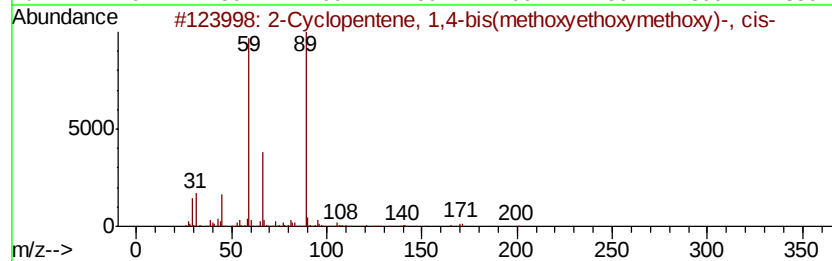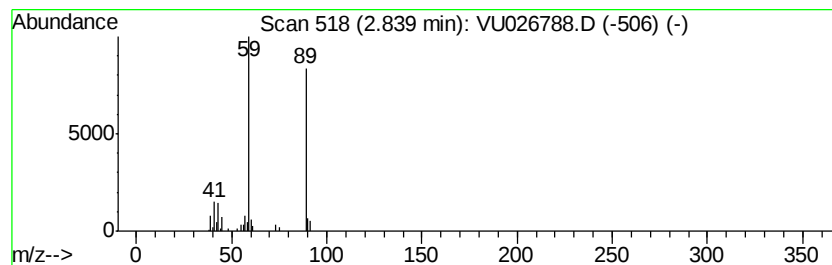

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU091618\
Data File : VU026788.D
Acq On : 15 Sep 2018 19:44
Operator : MD/SY
Sample : J4920-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KZ6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Cyclopentene, 1...	2.84	0.8	ug/L	45707	1	5.89	285784	5.0