


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
Data File : VU026768.D
Acq On : 15 Sep 2018 10:24
Operator : MD/SY
Sample : BFB40
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Sep 17 07:09:54 2018

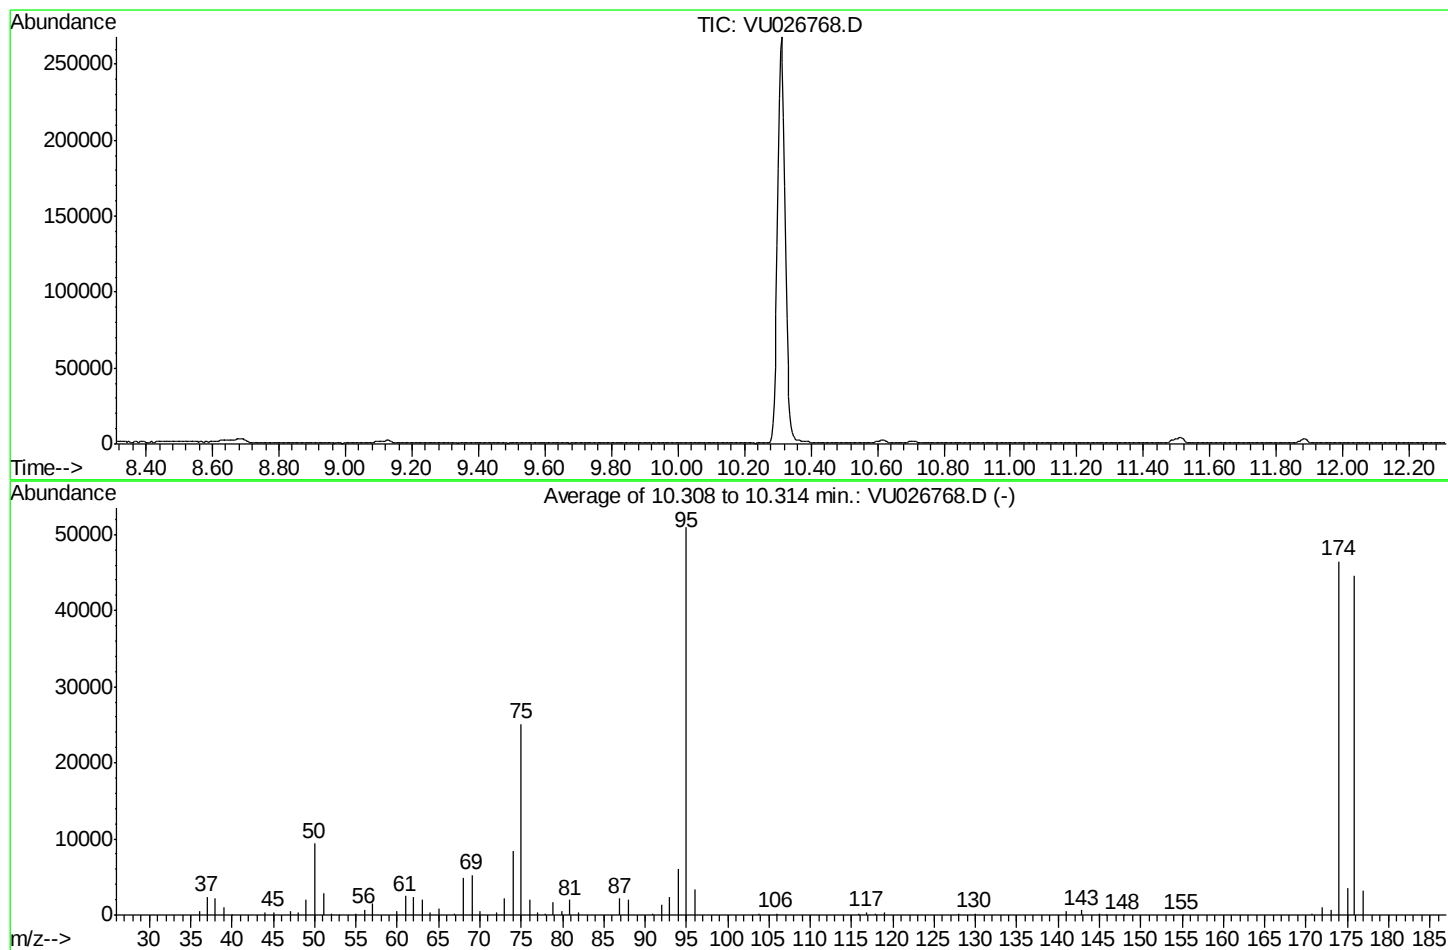

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	9348	PASS
75	95	30	80	49.2	25074	PASS
95	95	100	100	100.0	50941	PASS
96	95	5	9	6.8	3441	PASS
173	174	0.00	2	1.4	657	PASS
174	95	50	120	91.2	46445	PASS
175	174	5	9	7.8	3614	PASS
176	174	95	101	95.9	44538	PASS
177	176	5	9	7.1	3158	PASS

m/z	Abundance
39.90	121.0
44.00	519.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	504.0
37.00	2496.0
38.00	2237.0
39.00	1129.0
40.00	141.0
44.00	796.0
45.00	379.0
47.10	580.0
48.00	338.0
49.00	2075.0
50.00	9314.0
51.10	3105.0
52.00	180.0
55.00	143.0
56.00	799.0
57.00	1509.0
60.00	544.0
61.00	2649.0
62.00	2393.0
63.00	2065.0
64.00	404.0
65.00	796.0
66.90	190.0
68.00	4982.0
69.00	5384.0
70.00	427.0
72.00	305.0
73.00	2229.0
74.00	8380.0
75.00	25192.0
76.00	2127.0
76.90	324.0
77.90	207.0
78.90	1698.0
79.90	406.0
80.90	1952.0
81.90	366.0
86.90	2144.0
88.00	2130.0
90.90	211.0
92.00	1435.0
93.00	2400.0
94.00	6132.0
95.00	51424.0
96.00	3535.0
103.80	205.0
105.90	216.0
115.90	158.0
116.90	374.0
117.90	178.0
118.90	348.0
127.90	193.0
129.90	241.0
140.90	465.0
142.90	671.0
144.90	213.0
145.80	106.0
147.90	114.0
155.00	138.0
170.80	101.0
171.90	1041.0
173.00	690.0
174.00	45248.0
175.00	3513.0
175.90	43736.0
177.00	3195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	515.0
37.00	2449.0
38.00	2324.0
39.00	1080.0
40.10	132.0
44.00	775.0
45.00	402.0
47.10	565.0
48.00	294.0
49.00	2064.0
50.00	9635.0
51.00	3004.0
52.00	220.0
53.00	104.0
54.90	158.0
56.00	684.0
57.00	1512.0
60.00	548.0
61.00	2619.0
62.00	2405.0
63.00	2070.0
64.00	414.0
65.10	855.0
66.90	178.0
68.00	4963.0
69.00	5482.0
70.00	452.0
72.00	334.0
73.00	2265.0
74.00	8631.0
75.00	25960.0
76.00	2182.0
76.90	332.0
77.90	238.0
78.90	1747.0
79.90	451.0
80.90	2024.0
81.90	330.0
87.00	2180.0
88.00	2076.0
90.90	206.0
92.00	1457.0
93.00	2533.0
94.00	6299.0
95.00	52568.0
96.00	3550.0
103.80	227.0
105.90	250.0
115.90	199.0
116.90	400.0
117.90	202.0
118.90	331.0
127.90	199.0
129.90	257.0
140.90	529.0
142.90	650.0
144.90	219.0
145.90	111.0
147.90	110.0
155.00	124.0
170.80	128.0
171.90	1143.0
173.00	679.0
174.00	48000.0
175.00	3731.0
175.90	45968.0
177.00	3293.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	451.0
37.00	2250.0
38.00	2143.0
39.00	976.0
40.20	109.0
44.00	768.0
45.00	383.0
47.00	573.0
48.00	255.0
49.00	1892.0
50.00	9096.0
51.00	2690.0
52.00	199.0
53.00	109.0
54.90	173.0
56.00	554.0
57.00	1387.0
60.00	548.0
61.00	2295.0
62.00	2321.0
63.00	1937.0
64.00	389.0
65.10	790.0
66.90	142.0
68.00	4495.0
69.00	4931.0
70.00	438.0
72.00	336.0
73.00	2162.0
74.00	8098.0
75.00	24072.0
76.00	1994.0
77.00	320.0
77.80	237.0
78.90	1646.0
79.90	445.0
80.90	1906.0
81.90	318.0
87.00	2012.0
87.90	1888.0
90.90	169.0
92.00	1305.0
93.00	2359.0
94.00	5788.0
95.00	48832.0
96.00	3240.0
103.80	230.0
105.90	235.0
115.90	198.0
116.80	401.0
117.90	210.0
118.90	294.0
127.90	182.0
129.90	218.0
140.90	527.0
142.90	593.0
145.00	201.0
170.80	138.0
171.90	1099.0
173.10	603.0
174.00	46088.0
175.00	3598.0
175.90	43912.0
177.00	2986.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40