


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091618\
Data File : VU026812.D
Acq On : 17 Sep 2018 07:22
Operator : MD/SY
Sample : BFB41
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR091618WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Sep 17 07:09:54 2018

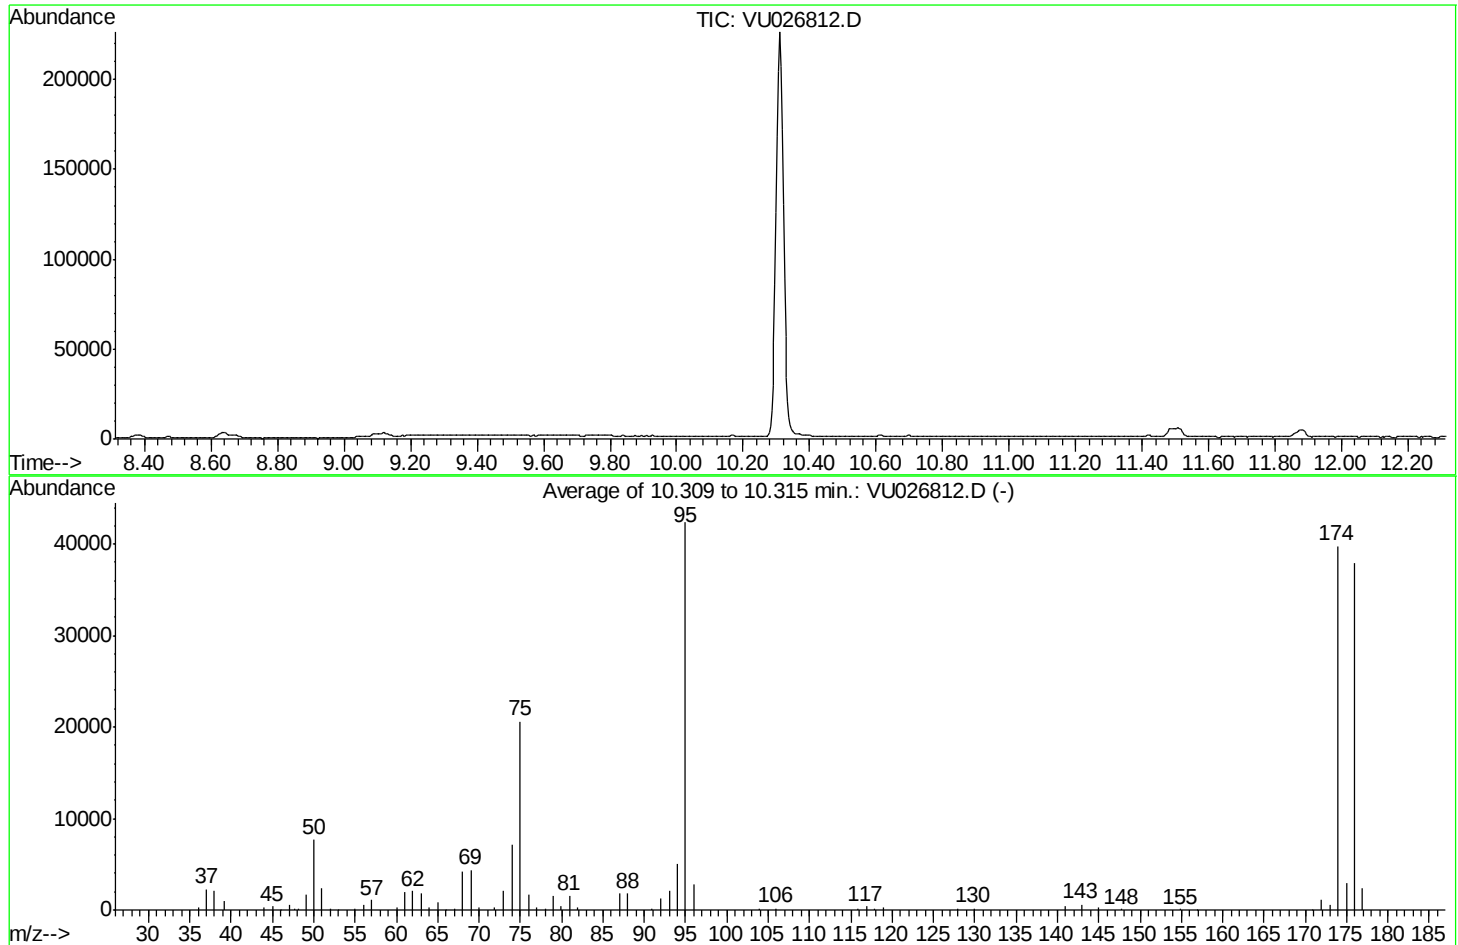

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	7671	PASS
75	95	30	80	48.6	20592	PASS
95	95	100	100	100.0	42368	PASS
96	95	5	9	6.5	2755	PASS
173	174	0.00	2	1.3	528	PASS
174	95	50	120	93.9	39784	PASS
175	174	5	9	7.2	2882	PASS
176	174	95	101	95.2	37869	PASS
177	176	5	9	6.4	2413	PASS

Scan 2828 (10.267 min): VU026812.D
BFB41

m/z	Abundance
36.00	793.0
37.80	274.0
44.00	433.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	1041.0
37.00	2423.0
38.00	2458.0
39.10	1021.0
44.00	638.0
45.00	422.0
45.90	106.0
47.00	642.0
48.10	213.0
49.00	1696.0
50.10	8167.0
51.00	2473.0
51.90	109.0
54.90	140.0
56.00	666.0
57.00	1111.0
60.00	305.0
61.00	2049.0
62.00	2202.0
63.00	2049.0
64.00	375.0
65.00	778.0
67.00	143.0
68.00	4435.0
69.00	4539.0
70.00	310.0
71.90	277.0
73.00	2106.0
74.00	7484.0
75.00	21520.0
76.00	1842.0
77.00	319.0
78.00	220.0
78.90	1601.0
79.90	439.0
80.90	1614.0
81.90	266.0
87.00	1726.0
88.00	1847.0
90.90	189.0
92.00	1328.0
93.00	2162.0
94.00	5237.0
95.00	43416.0
96.00	2934.0
103.80	119.0
106.00	198.0
115.90	149.0
116.90	460.0
117.90	244.0
118.90	329.0
127.90	111.0
129.90	174.0
141.00	440.0
142.90	624.0
144.90	222.0
147.80	113.0
154.90	103.0
156.90	102.0
171.90	1042.0
173.00	593.0
173.90	40000.0
175.00	2988.0
175.90	38216.0
177.00	2526.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	1032.0
37.00	2393.0
38.00	2371.0
39.10	1072.0
44.00	674.0
45.00	395.0
46.00	100.0
47.00	618.0
47.70	174.0
48.10	169.0
49.00	1705.0
50.10	7903.0
51.00	2425.0
52.00	112.0
54.90	139.0
56.00	667.0
57.00	1120.0
60.10	309.0
61.00	1996.0
62.00	2162.0
63.00	1847.0
64.00	355.0
65.10	822.0
67.00	118.0
68.00	4340.0
69.00	4493.0
70.00	300.0
71.90	260.0
73.00	2143.0
74.00	7290.0
75.00	21240.0
76.00	1715.0
77.00	289.0
78.00	219.0
78.90	1558.0
79.90	412.0
81.00	1623.0
81.90	284.0
87.00	1845.0
88.00	1877.0
90.90	192.0
92.00	1240.0
93.00	2110.0
94.00	5219.0
95.00	43840.0
96.00	2842.0
103.80	163.0
105.90	214.0
115.80	160.0
116.90	436.0
117.90	206.0
119.00	325.0
127.90	142.0
129.90	211.0
141.00	467.0
142.90	609.0
144.90	242.0
147.80	118.0
154.90	120.0
171.90	1110.0
173.00	541.0
173.90	40864.0
175.00	2940.0
175.90	39096.0
177.00	2477.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	1069.0
37.00	2075.0
38.00	2207.0
39.10	964.0
44.00	687.0
45.00	332.0
47.00	574.0
47.70	192.0
49.10	1665.0
50.00	6945.0
51.00	2154.0
52.00	120.0
53.00	103.0
55.00	111.0
56.00	559.0
57.00	1065.0
60.10	346.0
61.00	1784.0
62.00	1927.0
63.00	1574.0
64.00	314.0
65.10	791.0
65.90	109.0
68.00	3871.0
69.00	4169.0
70.00	270.0
71.90	223.0
73.00	1880.0
74.00	6604.0
75.00	19016.0
76.00	1457.0
76.90	270.0
78.00	197.0
78.90	1365.0
79.90	347.0
81.00	1515.0
81.90	276.0
87.00	1768.0
88.00	1648.0
91.00	170.0
92.00	1081.0
93.00	1908.0
94.10	4646.0
95.00	39848.0
96.00	2491.0
103.90	192.0
105.90	210.0
115.80	143.0
116.90	358.0
117.90	148.0
119.00	289.0
127.90	154.0
129.90	198.0
141.00	433.0
142.90	569.0
144.90	226.0
147.80	100.0
154.90	124.0
170.80	100.0
171.90	1140.0
173.00	452.0
173.90	38488.0
175.00	2718.0
175.90	36296.0
176.90	2236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41