
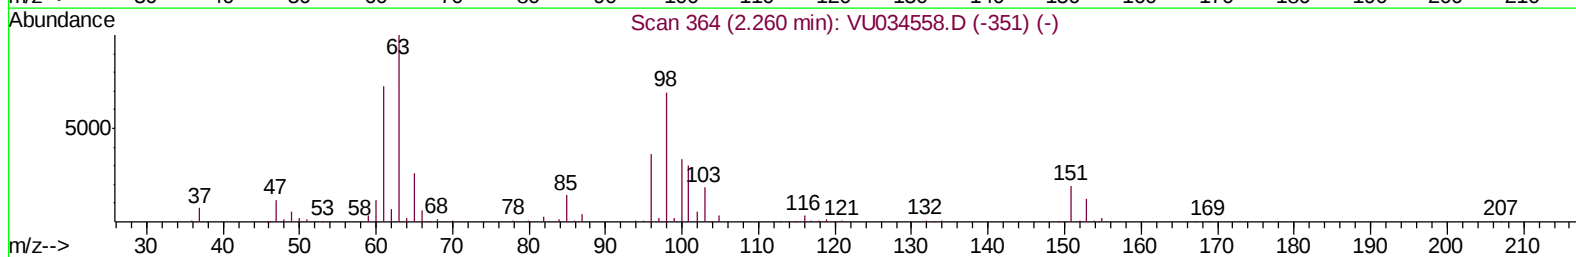
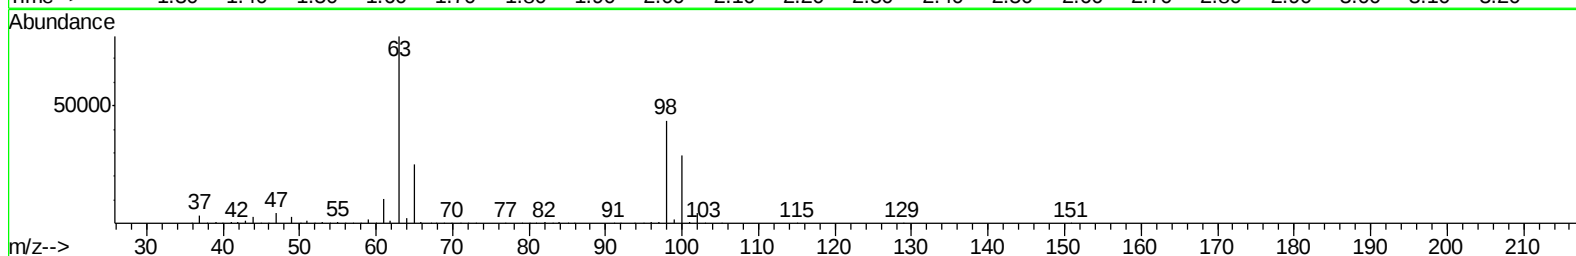


Data File : VU034564.D
Acq On : 16 Sep 2019 15:01
Operator : JC/SP
Sample : K4838-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Sep 17 03:57:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 17 02:36:09 2019
Response via : Initial Calibration

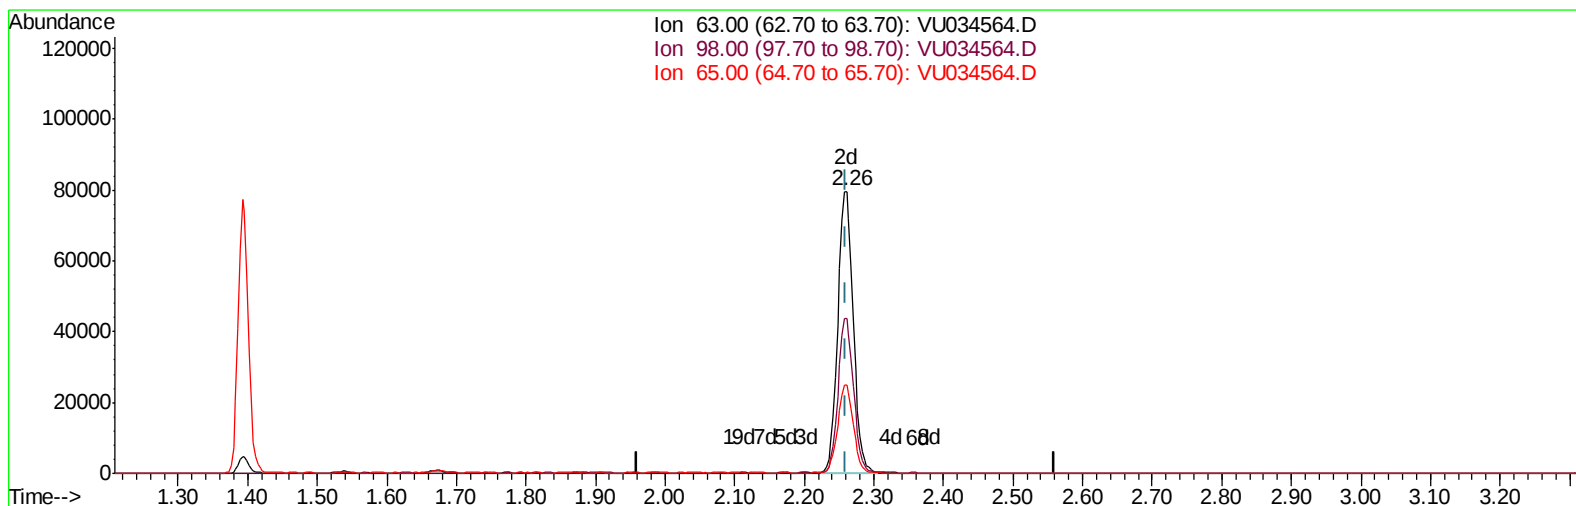

TIC: VU034564.D

(11) 1,1-Dichloroethene-d2 (S)

2.260min (-0.000) 36.39ug/L m

response 122545

Ion	Exp%	Act%
63.00	100	100
98.00	71.60	0.08#
65.00	23.70	0.02#
0.00	0.00	0.00