
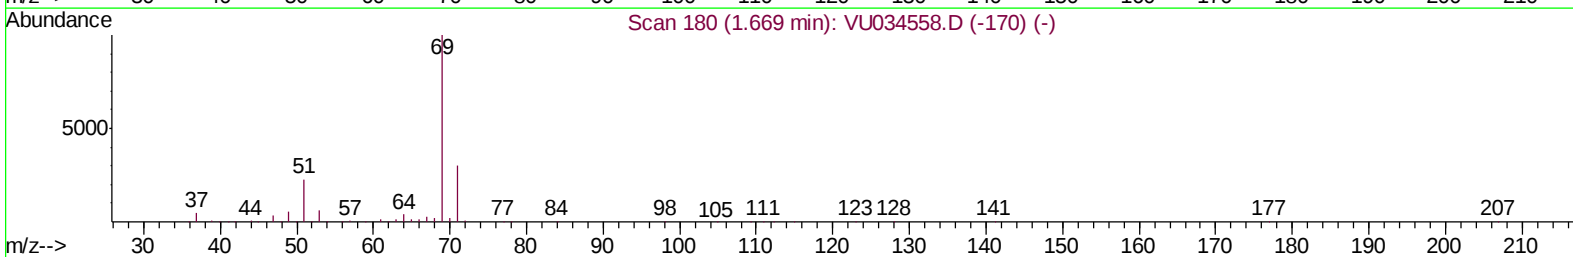
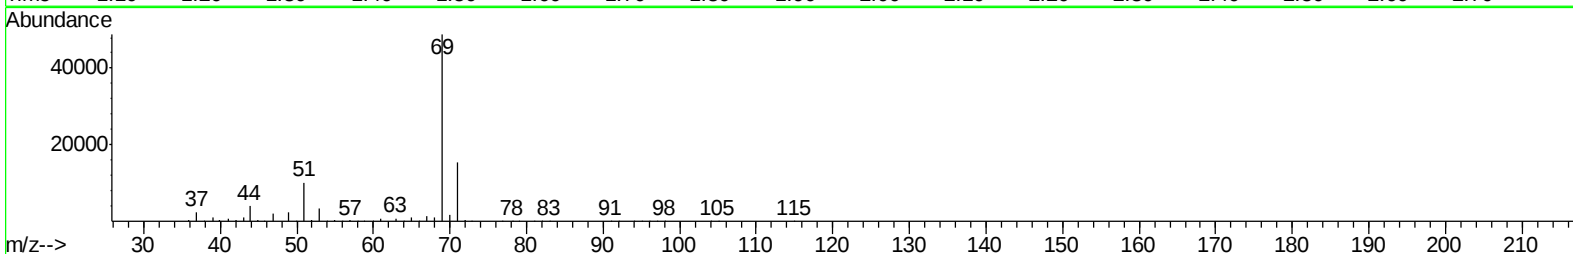


Data File : VU034575.D
Acq On : 16 Sep 2019 19:19
Operator : JC/SP
Sample : K4838-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Sep 17 02:59:18 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 17 02:36:09 2019
Response via : Initial Calibration

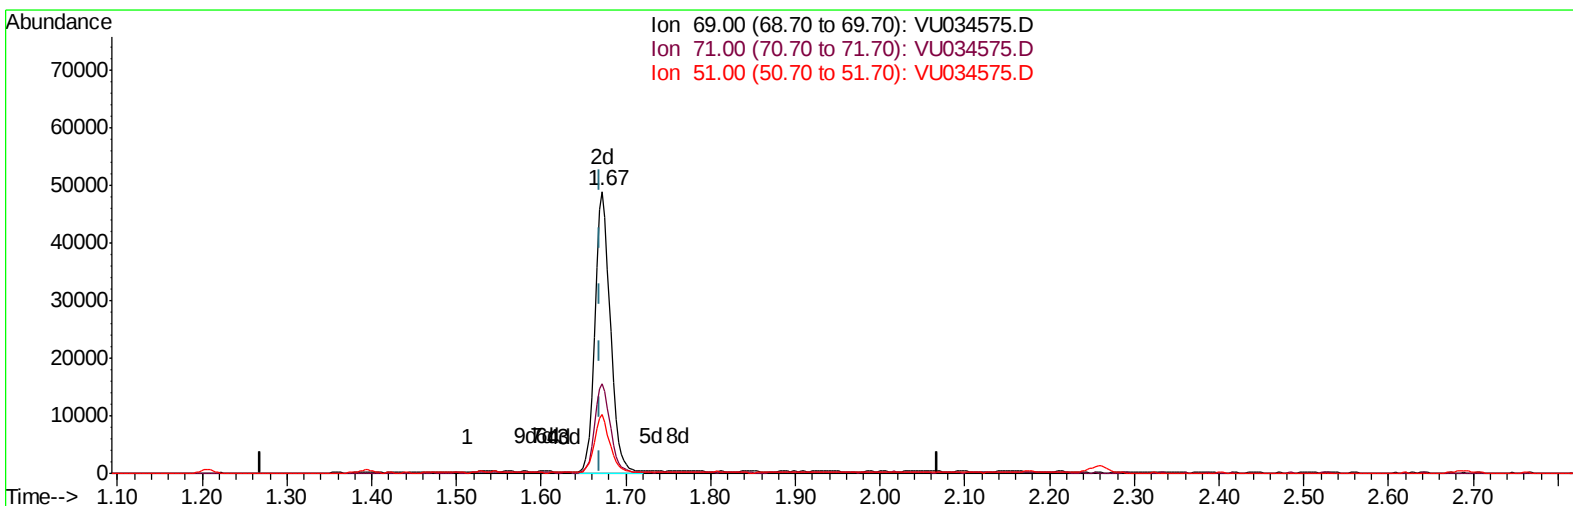

TIC: VU034575.D

(7) Chloroethane-d5 (S)

1.672min (+0.003) 54.61ug/L m

response 61734

Ion	Exp%	Act%
69.00	100	100
71.00	31.40	0.15#
51.00	31.10	0.14#
0.00	0.00	0.00