
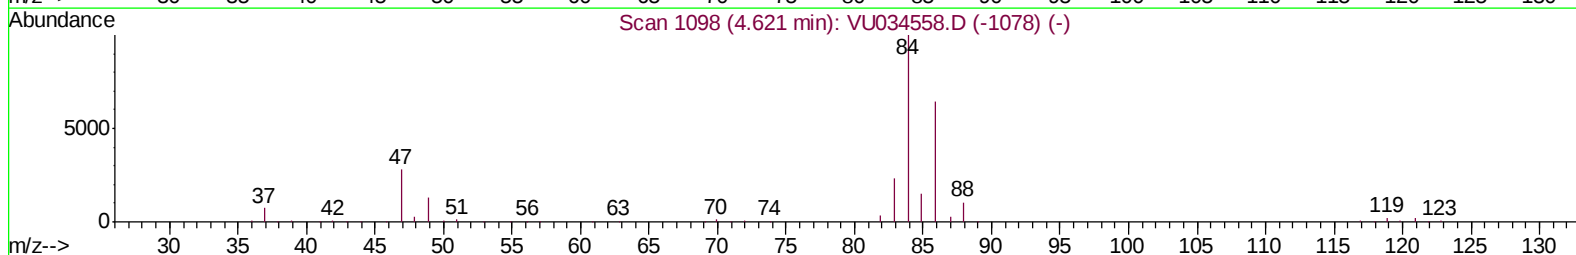
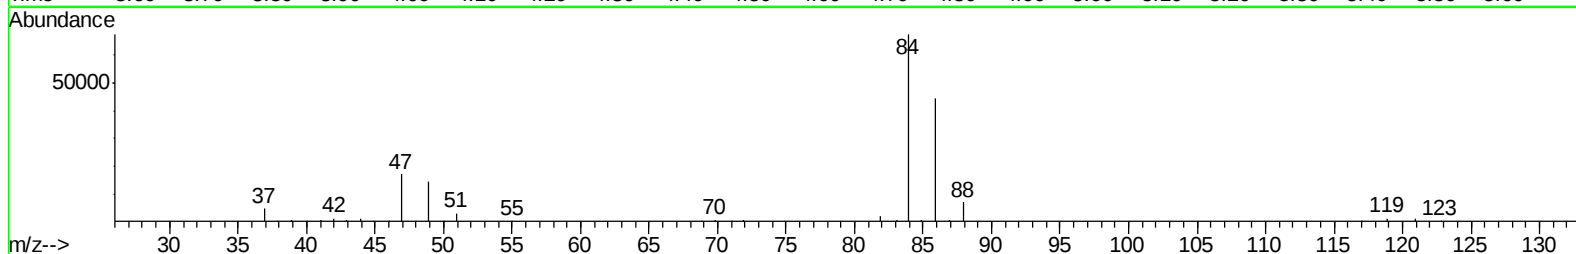


Data File : VU034579.D
Acq On : 16 Sep 2019 20:52
Operator : JC/SP
Sample : K4868-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Sep 17 02:59:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 17 02:36:09 2019
Response via : Initial Calibration

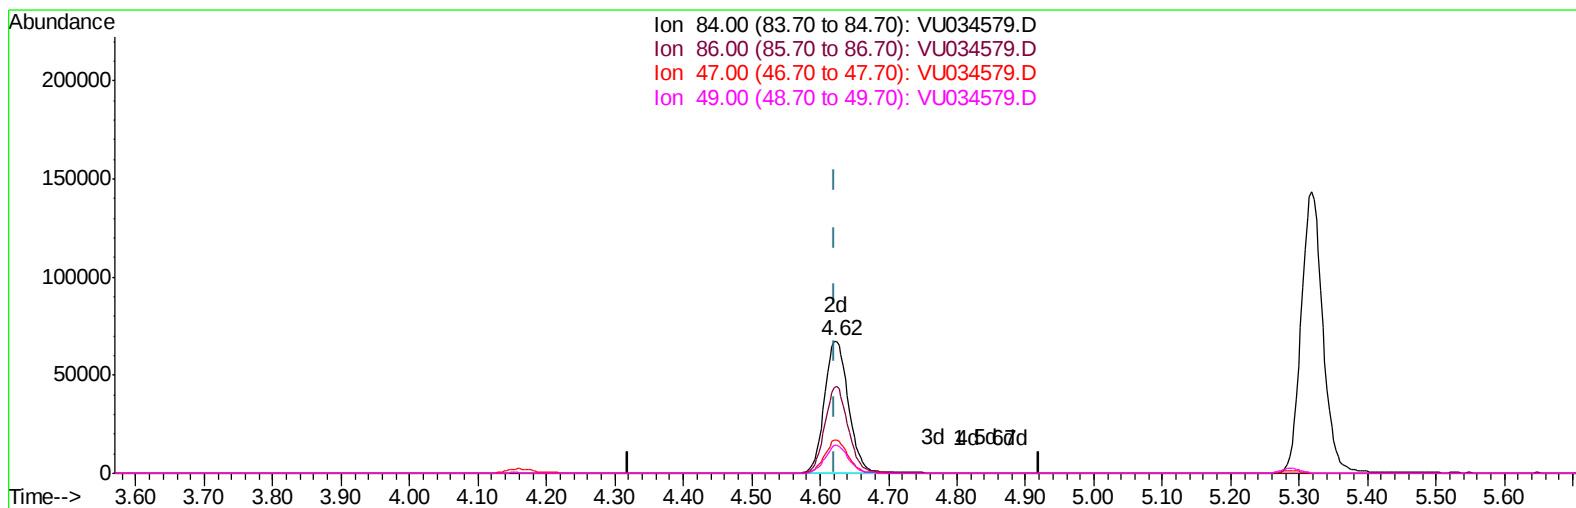

TIC: VU034579.D

(24) Chloroform-d (S)

4.624min (+0.003) 49.53ug/L m

response 163839

Ion	Exp%	Act%
84.00	100	100
86.00	63.00	0.05#
47.00	48.40	0.04#
49.00	28.60	0.03#