
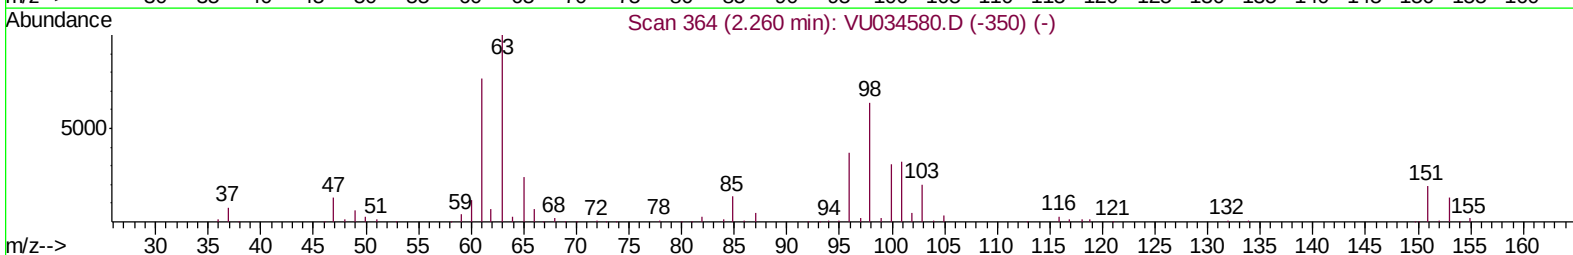
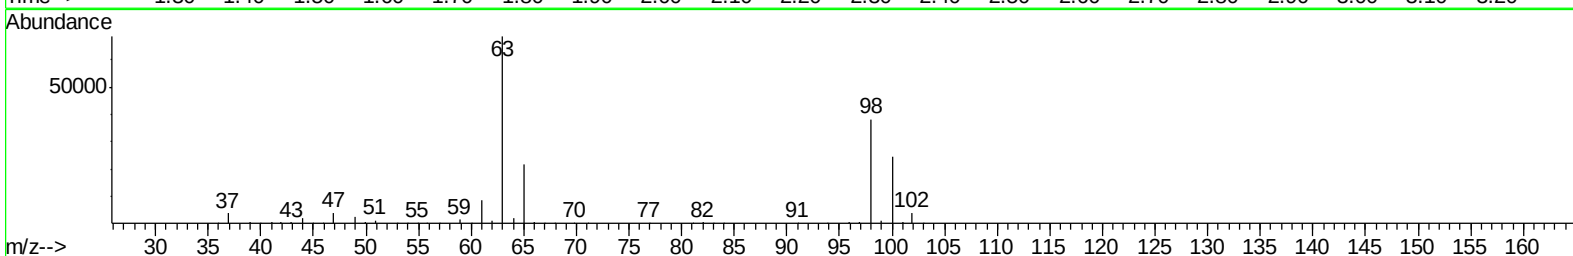


Data File : VU034581.D
Acq On : 16 Sep 2019 22:26
Operator : JC/SP
Sample : VU0916WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Sep 17 05:03:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 17 05:01:24 2019
Response via : Initial Calibration

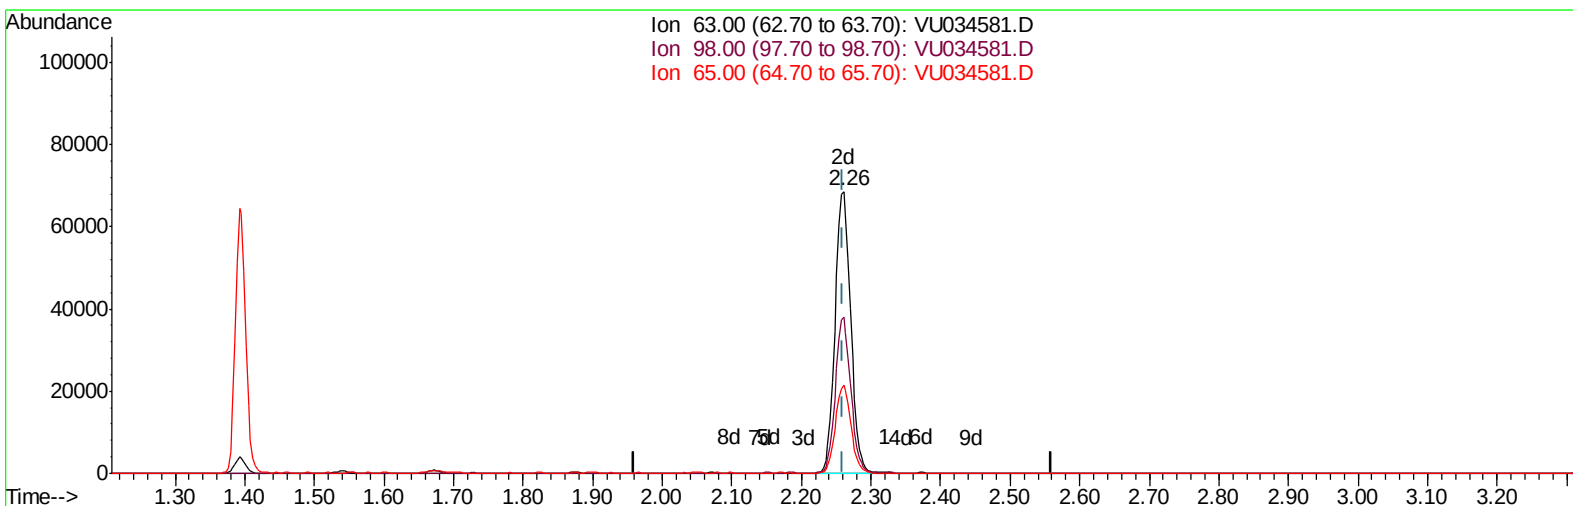

TIC: VU034581.D

(11) 1,1-Dichloroethene-d2 (S)

2.260min (-0.000) 38.74ug/L m

response 106821

Ion	Exp%	Act%
63.00	100	100
98.00	71.60	0.17#
65.00	23.70	0.07#
0.00	0.00	0.00