
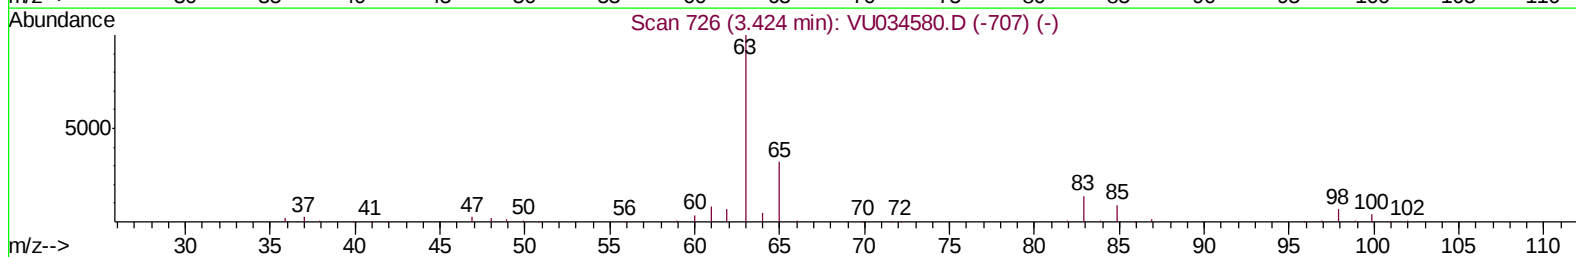
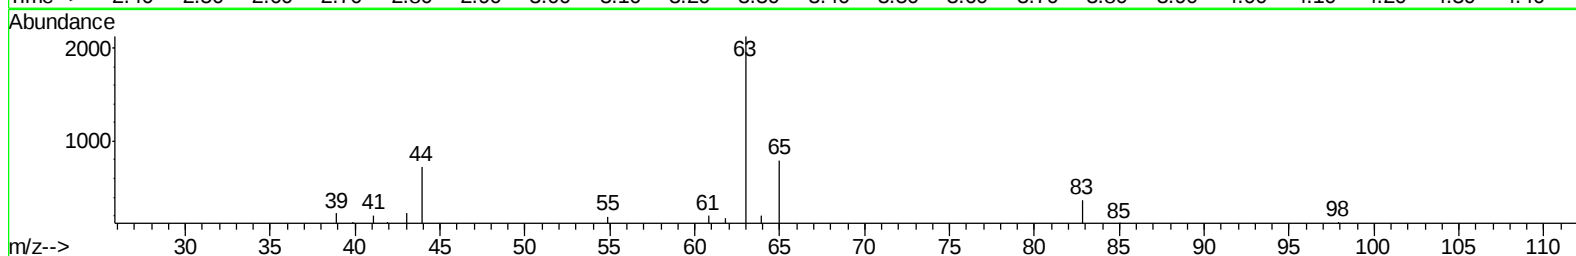


Data File : VU034590.D
Acq On : 17 Sep 2019 01:57
Operator : JC/SP
Sample : K4838-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Sep 17 05:05:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 17 05:01:24 2019
Response via : Initial Calibration

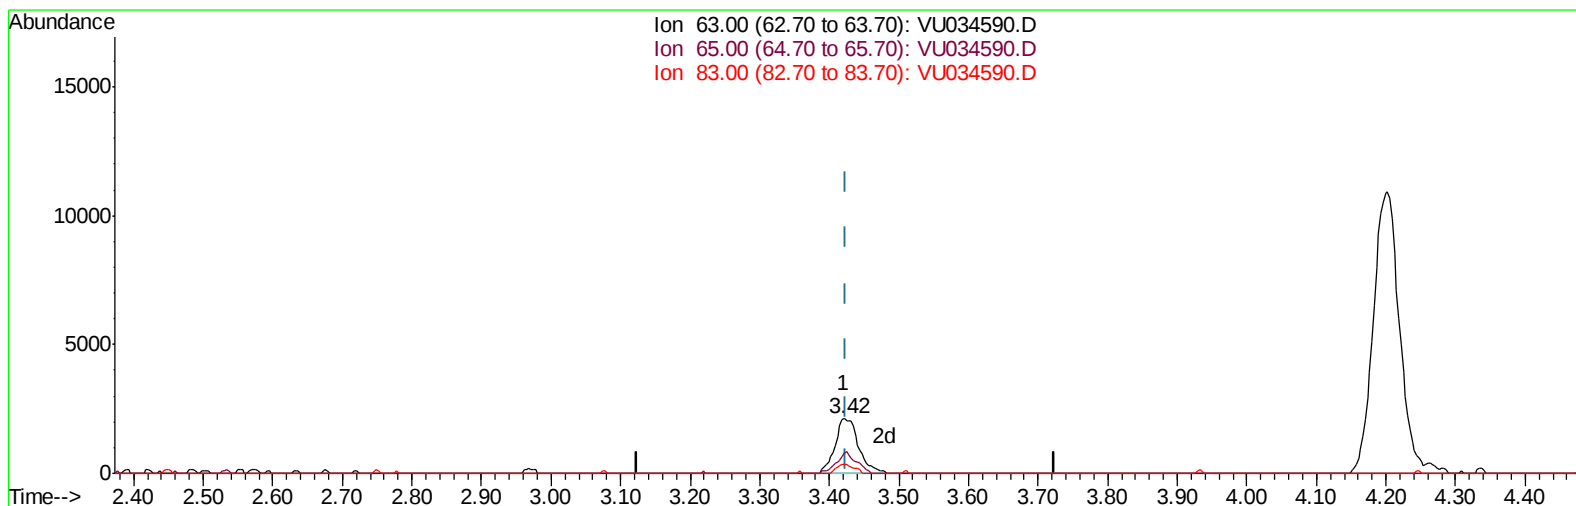

TIC: VU034590.D

(19) 1,1-Dichloroethane (T)

3.421min (-0.003) 1.60ug/L m

response 4944

Ion	Exp%	Act%
63.00	100	100
65.00	30.80	37.41
83.00	13.80	17.29
0.00	0.00	0.00