
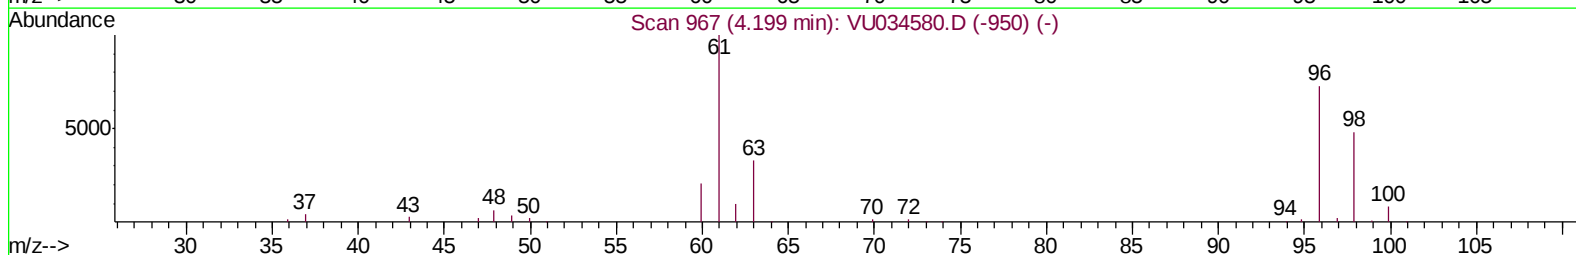
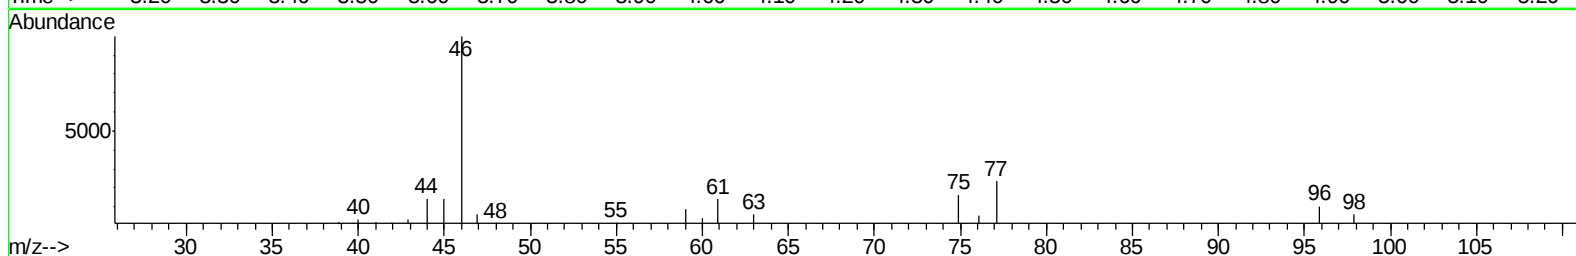


Data File : VU034593.D
Acq On : 17 Sep 2019 03:07
Operator : JC/SP
Sample : K4838-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Sep 17 05:06:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 17 05:01:24 2019
Response via : Initial Calibration

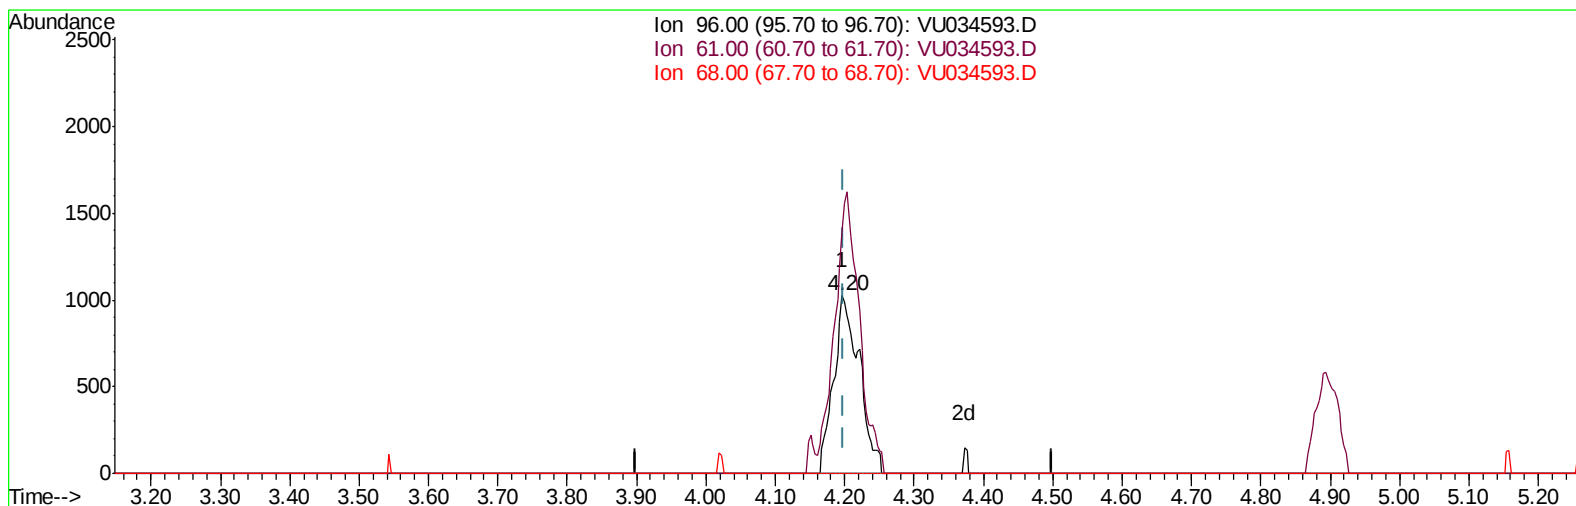

TIC: VU034593.D

(20) cis-1,2-Dichloroethene (T)

4.196min (-0.003) 1.52ug/L m

response 2646

Ion	Exp%	Act%
96.00	100	100
61.00	135.30	135.51
68.00	0.00	0.00
0.00	0.00	0.00