

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091619\
 Data File : VU034574.D
 Acq On : 16 Sep 2019 18:55
 Operator : JC/SP
 Sample : K4838-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0MD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	88	94	105	rBV	115741	121149	11.72%	1.383%
2	1.672	175	181	194	rVB	91983	114256	11.06%	1.305%
3	2.257	356	363	377	rVB	207035	313574	30.34%	3.581%
4	2.997	591	593	597	rBV4	678	541	0.05%	0.006%
5	3.019	598	600	603	rVV2	965	574	0.06%	0.007%
6	3.071	613	616	617	rBV2	522	271	0.03%	0.003%
7	3.100	624	625	627	rVB2	445	114	0.01%	0.001%
8	3.138	635	637	638	rBV2	391	220	0.02%	0.003%
9	3.186	647	652	653	rBV3	606	397	0.04%	0.005%
10	3.309	687	690	693	rBV4	484	412	0.04%	0.005%
11	3.466	737	739	742	rBV3	734	428	0.04%	0.005%
12	3.485	743	745	749	rVB4	964	429	0.04%	0.005%
13	3.502	749	750	751	rVB	293	56	0.01%	0.001%
14	3.514	751	754	756	rBV3	725	495	0.05%	0.006%
15	3.559	765	768	769	rBV2	707	373	0.04%	0.004%
16	3.595	777	779	782	rVB3	565	291	0.03%	0.003%
17	3.608	782	783	784	rBV	611	214	0.02%	0.002%
18	3.682	805	806	808	rBV2	388	181	0.02%	0.002%
19	3.707	812	814	817	rVB3	716	356	0.03%	0.004%
20	3.739	821	824	830	rVB6	1122	1059	0.10%	0.012%
21	3.781	834	837	838	rBV2	733	399	0.04%	0.005%
22	3.810	845	846	850	rVB3	968	383	0.04%	0.004%
23	3.829	850	852	854	rBV	294	181	0.02%	0.002%
24	3.852	854	859	861	rBV4	592	635	0.06%	0.007%
25	3.942	884	887	891	rVB3	1106	871	0.08%	0.010%
26	3.961	891	893	895	rVB2	384	159	0.02%	0.002%
27	3.977	895	898	900	rBV3	448	297	0.03%	0.003%
28	4.045	916	919	924	rVB6	836	726	0.07%	0.008%
29	4.074	924	928	929	rBV2	347	197	0.02%	0.002%
30	4.151	941	952	983	rBV3	126986	373667	36.16%	4.267%
31	4.624	1084	1099	1119	rBV	179608	422045	40.84%	4.819%
32	4.855	1165	1171	1173	rBV5	1425	1568	0.15%	0.018%
33	4.939	1194	1197	1200	rBV5	945	879	0.09%	0.010%
34	5.016	1216	1221	1224	rBV4	1042	931	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091619\
 Data File : VU034574.D
 Acq On : 16 Sep 2019 18:55
 Operator : JC/SP
 Sample : K4838-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0MD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis

35	5.080	1237	1241	1243	rBV3	420	231	0.02%	0.003%
36	5.090	1243	1244	1245	rBV	187	43	0.00%	0.000%
37	5.103	1245	1248	1251	rBV3	697	471	0.05%	0.005%
38	5.167	1265	1268	1270	rBV2	198	114	0.01%	0.001%
39	5.183	1270	1273	1275	rBV2	783	461	0.04%	0.005%
40	5.196	1275	1277	1281	rBV5	497	391	0.04%	0.004%
41	5.218	1281	1284	1287	rVB2	1031	654	0.06%	0.007%
42	5.315	1287	1314	1339	rBV2	342096	1033434	100.00%	11.801%
43	5.720	1435	1440	1441	rBV4	1293	1056	0.10%	0.012%
44	5.775	1456	1457	1459	rVB2	608	130	0.01%	0.001%
45	5.807	1465	1467	1471	rVB5	915	487	0.05%	0.006%
46	5.865	1472	1485	1504	rBV	368252	739897	71.60%	8.449%
47	6.308	1611	1623	1645	rVB	255310	510796	49.43%	5.833%
48	7.099	1866	1869	1871	rBV3	750	384	0.04%	0.004%
49	7.206	1892	1902	1928	rBV	143224	271788	26.30%	3.104%
50	7.543	1994	2007	2027	rBV	476931	845238	81.79%	9.652%
51	7.829	2086	2096	2121	rBV	99536	185963	17.99%	2.123%
52	8.041	2159	2162	2168	rBV7	1280	1482	0.14%	0.017%
53	8.160	2190	2199	2209	rBV3	4000	7083	0.69%	0.081%
54	8.292	2228	2240	2275	rBV	348548	683901	66.18%	7.809%
55	8.627	2339	2344	2349	rBV7	899	1152	0.11%	0.013%
56	8.781	2387	2392	2397	rVB4	1066	920	0.09%	0.011%
57	8.816	2397	2403	2405	rBV5	657	712	0.07%	0.008%
58	9.067	2469	2481	2514	rBV	535490	914656	88.51%	10.444%
59	9.360	2569	2572	2577	rBV5	1022	1145	0.11%	0.013%
60	9.408	2582	2587	2590	rBV4	1128	893	0.09%	0.010%
61	9.443	2595	2598	2600	rBV3	704	458	0.04%	0.005%
62	9.466	2603	2605	2606	rBV	458	166	0.02%	0.002%
63	9.582	2638	2641	2645	rBV4	828	422	0.04%	0.005%
64	9.617	2649	2652	2654	rBV5	967	473	0.05%	0.005%
65	9.649	2659	2662	2665	rBV4	709	416	0.04%	0.005%
66	9.868	2728	2730	2732	rBV3	949	494	0.05%	0.006%
67	9.996	2766	2770	2773	rBV4	981	919	0.09%	0.010%
68	10.106	2803	2804	2805	rBV	467	178	0.02%	0.002%
69	10.131	2808	2812	2813	rBV2	556	385	0.04%	0.004%
70	10.202	2831	2834	2839	rVB4	1047	787	0.08%	0.009%
71	10.228	2839	2842	2844	rBV3	1021	619	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091619\
 Data File : VU034574.D
 Acq On : 16 Sep 2019 18:55
 Operator : JC/SP
 Sample : K4838-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0MD1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis

72	10.308	2863	2867	2869	rBV3	1150	983	0.10%	0.011%
73	10.408	2885	2898	2919	rBV	369680	609088	58.94%	6.955%
74	10.591	2947	2955	2963	rBV8	3096	4512	0.44%	0.052%
75	10.816	3023	3025	3027	rBV3	831	387	0.04%	0.004%
76	10.897	3048	3050	3052	rBV3	677	375	0.04%	0.004%
77	11.135	3121	3124	3125	rBV2	1080	581	0.06%	0.007%
78	11.395	3201	3205	3207	rBV4	957	870	0.08%	0.010%
79	11.459	3214	3225	3245	rBV	469678	793301	76.76%	9.059%
80	11.836	3330	3342	3361	rBV	459664	774379	74.93%	8.843%
81	12.533	3557	3559	3567	rVB6	2011	1827	0.18%	0.021%
82	12.572	3567	3571	3573	rBV3	1085	954	0.09%	0.011%
83	12.749	3624	3626	3632	rBV4	1111	1106	0.11%	0.013%
84	13.295	3792	3796	3798	rBV2	1153	959	0.09%	0.011%
85	13.829	3959	3962	3965	rBV4	1450	973	0.09%	0.011%


Sum of corrected areas: 8757422

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091619\
Data File : VU034574.D
Acq On : 16 Sep 2019 18:55
Operator : JC/SP
Sample : K4838-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

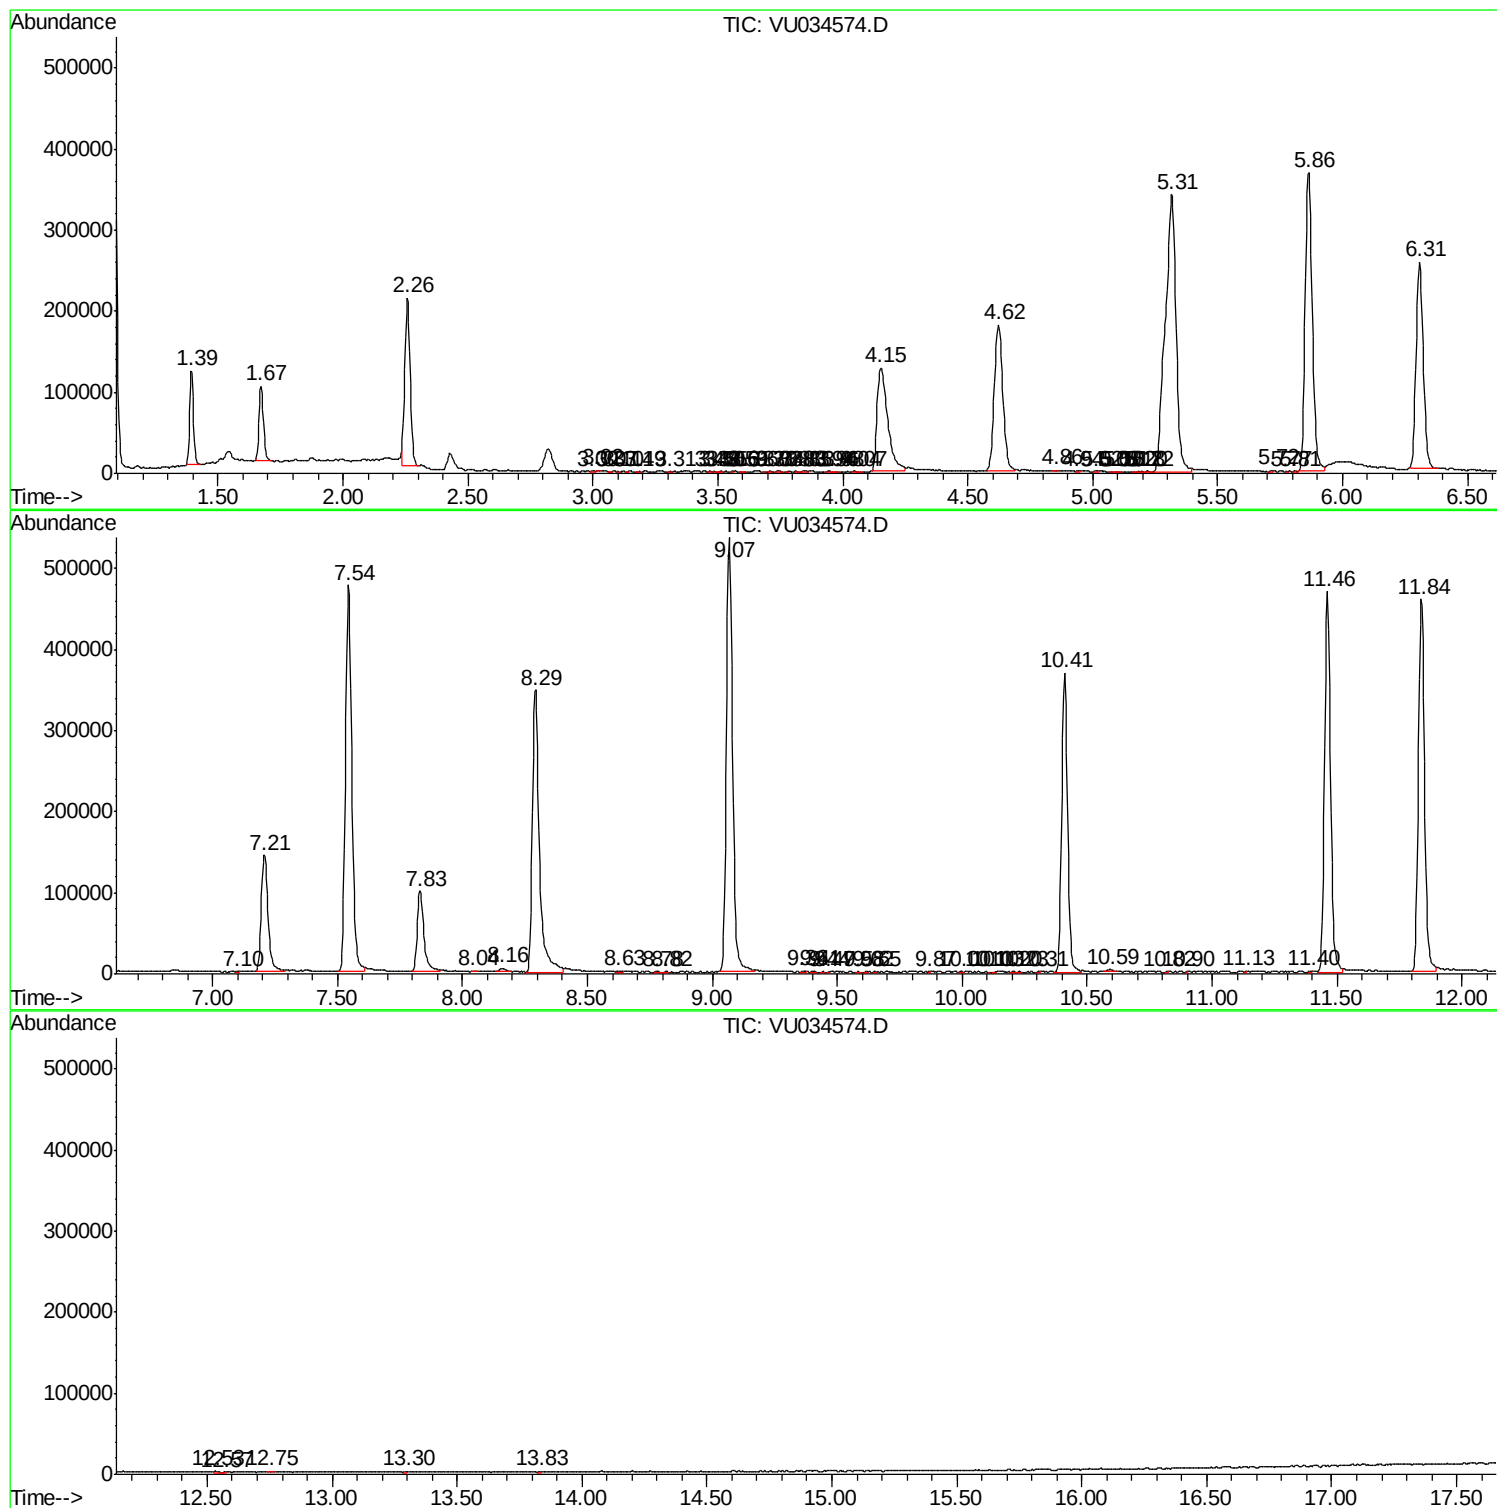

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091619\
Data File : VU034574.D
Acq On : 16 Sep 2019 18:55
Operator : JC/SP
Sample : K4838-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU091619\
Data File : VU034574.D
Acq On : 16 Sep 2019 18:55
Operator : JC/SP
Sample : K4838-11
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0MD1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
