


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091619\
 Data File : VU034555.D
 Acq On : 16 Sep 2019 10:10
 Operator : JC/SP
 Sample : BFB32
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB32

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 16 12:37:26 2019

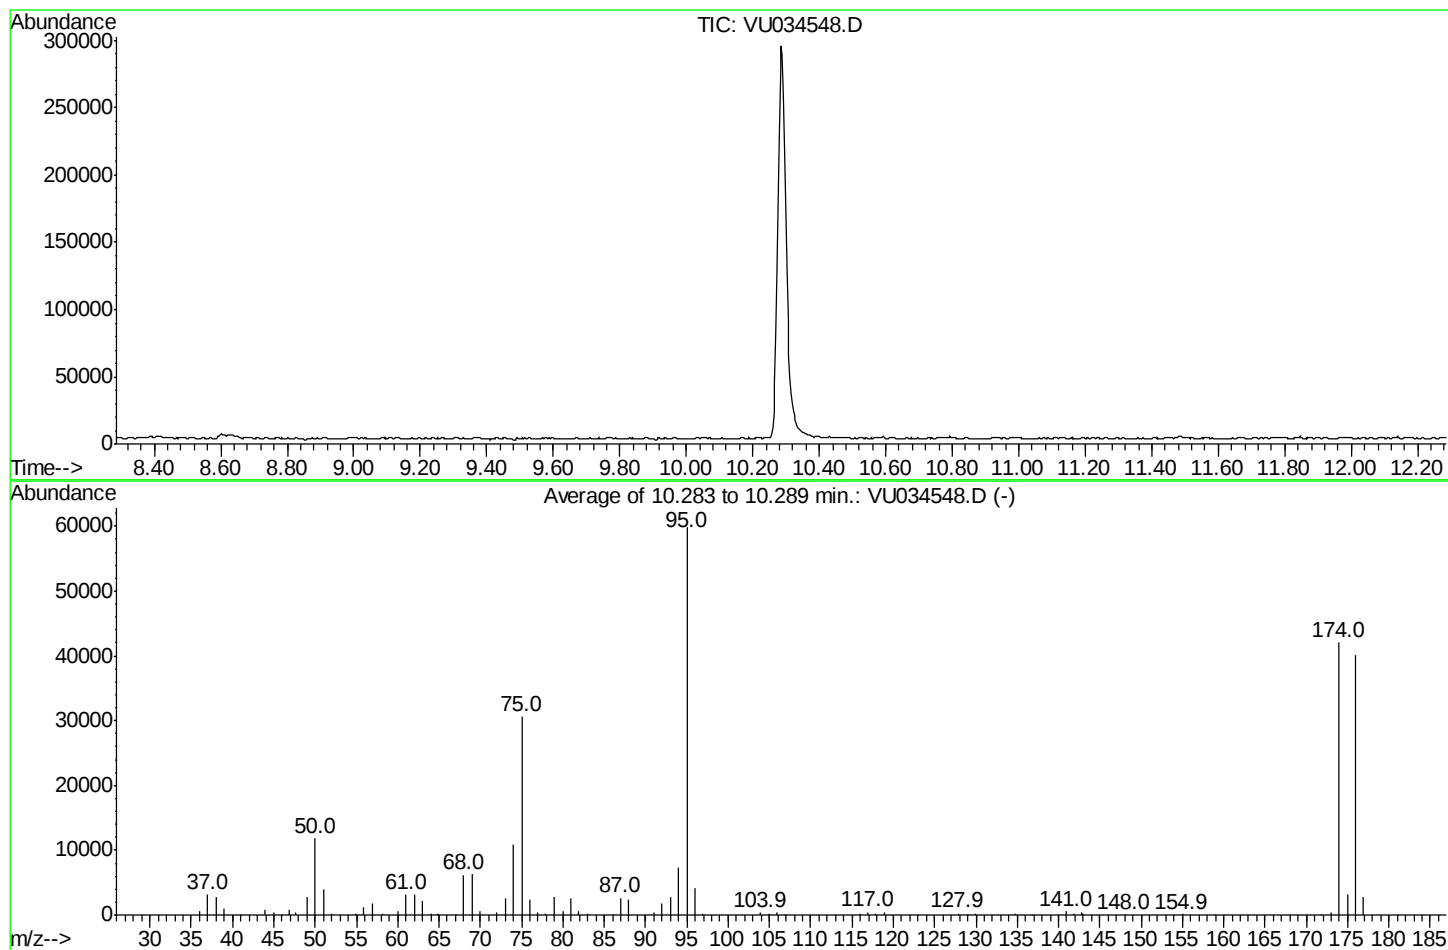

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	11791	PASS
75	95	30	80	51.2	30621	PASS
95	95	100	100	100.0	59840	PASS
96	95	5	9	6.9	4103	PASS
173	174	0.00	2	1.1	471	PASS
174	95	50	120	70.2	42005	PASS
175	174	5	9	7.5	3156	PASS
176	174	95	101	95.6	40141	PASS
177	176	5	9	7.0	2812	PASS

m/z	Abundance
35.90	589.0
37.00	3081.0
38.00	2936.0
39.10	1133.0
39.90	310.0
40.90	422.0
41.90	136.0
43.00	404.0
44.00	1712.0
45.10	661.0
46.90	726.0
47.70	374.0
49.00	2861.0
50.00	11766.0
51.00	3931.0
52.00	251.0
53.90	129.0
54.90	406.0
55.90	1201.0
57.00	1994.0
58.00	205.0
60.00	620.0
61.00	3095.0
62.00	3111.0
63.00	2138.0
64.00	239.0
64.80	107.0
67.10	237.0
68.00	6074.0
69.00	6222.0
70.00	689.0
71.00	171.0
71.90	322.0
73.00	2431.0
74.00	10753.0
75.00	29768.0
76.00	2243.0
76.90	473.0
77.80	257.0
78.90	2781.0
80.00	685.0
80.90	2470.0
81.90	589.0
82.90	113.0
87.00	2752.0
88.00	2497.0
90.90	362.0
92.00	1631.0
93.00	2680.0
94.00	7028.0
95.00	56728.0
96.00	4168.0
96.80	104.0
103.90	403.0
104.90	139.0
105.90	335.0
106.90	127.0
116.00	236.0
117.00	454.0
117.90	256.0
118.90	380.0
127.90	261.0
129.00	113.0
129.80	168.0
134.80	179.0
136.80	100.0
141.00	449.0
141.90	103.0
142.80	483.0
148.00	126.0
155.00	122.0
172.90	408.0
174.00	39560.0
175.00	2882.0
176.00	38224.0
176.90	2696.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	619.0
37.00	3212.0
38.00	2933.0
39.00	1305.0
39.90	286.0
41.00	439.0
41.90	183.0
43.00	386.0
44.00	1879.0
45.10	641.0
45.90	103.0
46.90	806.0
47.70	391.0
49.00	2858.0
50.00	12146.0
51.00	4060.0
52.00	270.0
53.90	109.0
55.00	426.0
55.90	1333.0
56.90	2115.0
58.10	169.0
60.00	726.0
61.00	3229.0
62.00	3337.0
63.00	2207.0
64.00	240.0
64.90	123.0
67.10	217.0
68.00	6418.0
69.00	6601.0
70.00	642.0
71.00	145.0
71.90	363.0
73.00	2701.0
74.00	11313.0
75.00	31472.0
76.00	2587.0
76.90	535.0
77.80	301.0
78.90	2728.0
79.90	685.0
80.90	2656.0
81.90	616.0
82.90	112.0
86.90	2569.0
88.00	2517.0
90.90	350.0
92.00	1724.0
93.00	2803.0
94.00	7534.0
95.00	61696.0
96.00	4260.0
96.90	150.0
103.90	404.0
105.00	147.0
105.90	332.0
116.00	265.0
116.90	465.0
117.90	237.0
118.90	430.0
127.90	254.0
129.80	152.0
134.80	187.0
141.00	547.0
141.80	131.0
142.80	496.0
154.90	135.0
172.90	477.0
174.00	43400.0
175.00	3215.0
176.00	41280.0
177.00	2979.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
35.90	620.0
37.00	3142.0
38.00	2697.0
39.00	1423.0
39.90	262.0
40.90	402.0
41.90	232.0
43.00	438.0
44.00	1728.0
45.10	585.0
45.90	101.0
46.90	893.0
47.70	361.0
49.00	2604.0
50.00	11463.0
51.00	3673.0
52.00	199.0
55.00	411.0
55.90	1351.0
56.90	1979.0
58.20	104.0
60.00	736.0
61.00	3079.0
62.00	3071.0
63.00	2174.0
64.00	216.0
64.90	112.0
67.00	212.0
68.00	6317.0
69.00	6373.0
70.00	560.0
71.00	104.0
72.00	410.0
73.00	2776.0
74.00	10738.0
75.00	30624.0
75.90	2584.0
76.90	487.0
77.80	299.0
78.90	2531.0
80.00	701.0
80.90	2700.0
81.90	617.0
82.90	140.0
86.00	107.0
86.90	2445.0
88.00	2332.0
91.00	309.0
92.00	1721.0
93.00	2598.0
94.00	7335.0
95.00	61096.0
96.00	3883.0
97.00	205.0
103.90	332.0
105.00	141.0
105.80	343.0
115.90	284.0
116.90	406.0
117.90	242.0
118.80	489.0
127.90	204.0
129.90	136.0
134.80	152.0
141.00	570.0
141.80	105.0
143.00	497.0
154.90	136.0
158.90	100.0
171.80	101.0
173.00	528.0
174.00	43056.0
174.90	3373.0
176.00	40920.0
177.00	2763.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
38.90	266.0
40.00	297.0
41.00	365.0
41.90	259.0
42.90	514.0
43.90	1071.0
44.90	132.0
52.90	101.0
54.10	103.0
55.00	299.0
56.00	163.0
57.00	207.0
60.10	113.0
67.10	126.0
68.10	126.0
69.20	118.0
69.90	126.0
71.00	158.0
80.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32