


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091620\
 Data File : VU040141.D
 Acq On : 16 Sep 2020 09:50
 Operator : SY/MD
 Sample : BFB02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB02

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Sep 17 02:07:00 2020

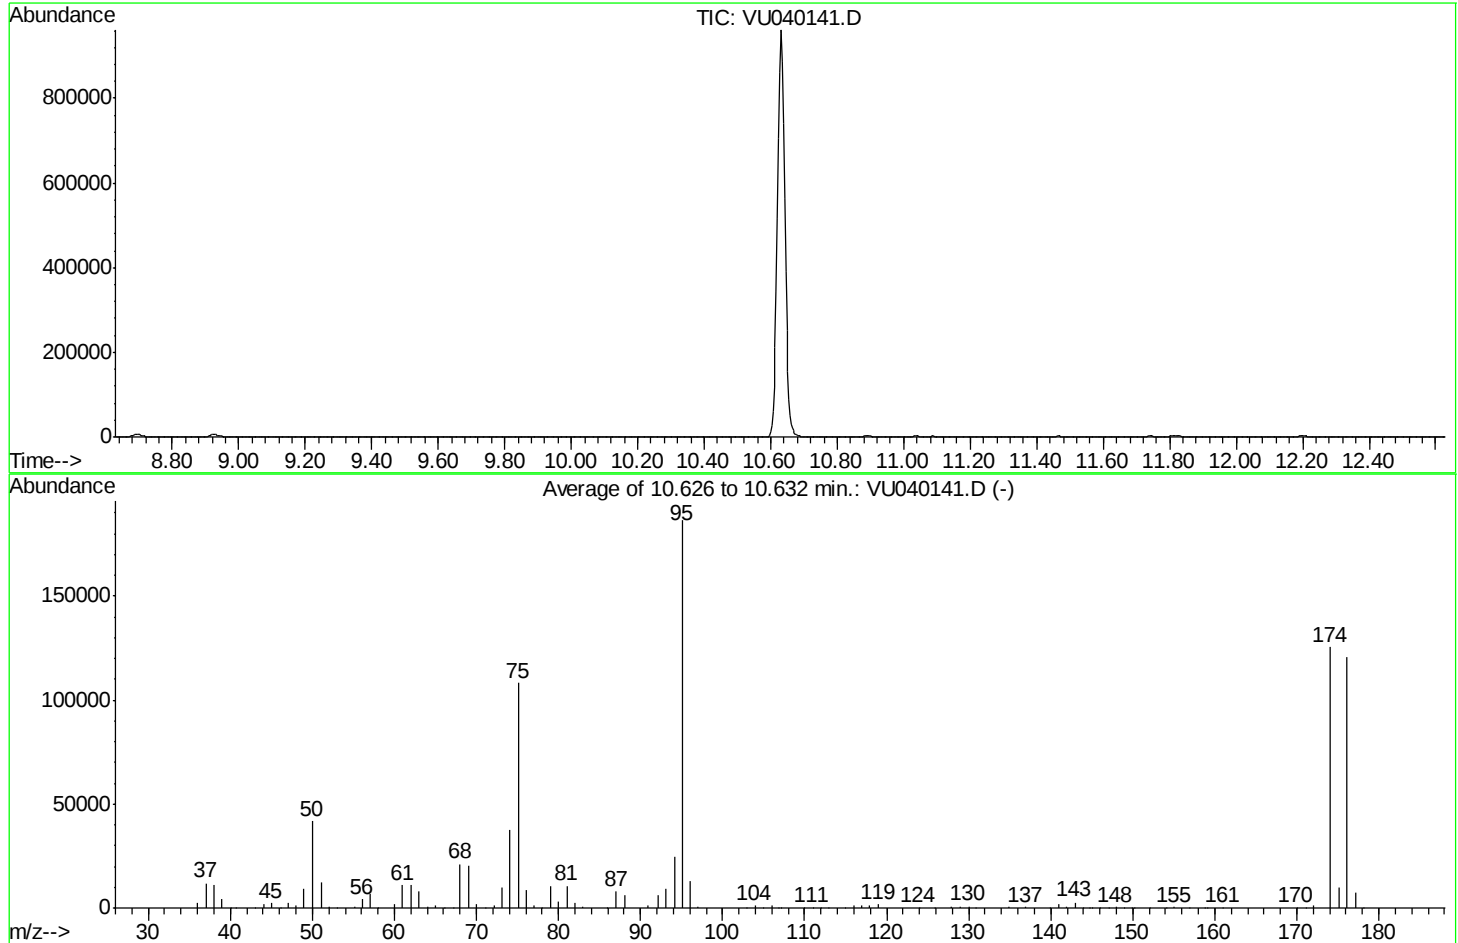

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	41714	PASS
75	95	30	80	58.1	108344	PASS
95	95	100	100	100.0	186496	PASS
96	95	5	9	6.8	12721	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.3	125594	PASS
175	174	5	9	7.7	9619	PASS
176	174	95	101	96.1	120674	PASS
177	176	5	9	6.2	7441	PASS

m/z	Abundance
36.00	2097.0
37.00	11594.0
38.00	10508.0
39.00	4359.0
40.00	309.0
40.70	152.0
43.00	119.0
44.10	1559.0
45.00	2075.0
46.20	197.0
47.00	2394.0
48.00	1387.0
49.00	8644.0
50.00	39176.0
51.10	12076.0
52.00	595.0
53.00	151.0
55.10	976.0
56.00	4028.0
57.00	6622.0
58.00	228.0
60.10	2173.0
61.00	10443.0
62.10	10667.0
63.00	7799.0
64.00	899.0
65.00	1202.0
66.10	133.0
67.10	400.0
68.00	19488.0
69.10	18560.0
70.00	1635.0
72.10	1049.0
73.10	9180.0
74.10	35464.0
75.10	100888.0
76.10	8248.0
77.00	1096.0
78.00	780.0
79.00	9865.0
80.00	2627.0
81.00	9746.0
82.00	2174.0
83.00	341.0
86.00	237.0
87.10	7283.0
88.10	6084.0
90.90	935.0
92.10	5544.0
93.10	8948.0
94.10	23424.0
95.10	174848.0
96.10	12061.0
97.00	354.0
102.90	120.0
104.00	1135.0
105.00	248.0
106.00	892.0
106.90	182.0
110.00	148.0
111.00	230.0
112.00	169.0
112.90	268.0
114.90	244.0
116.00	953.0
117.00	1247.0
117.90	1100.0
119.00	1621.0
124.00	144.0
127.90	673.0
129.10	307.0
130.00	870.0
130.90	198.0
134.80	278.0
136.90	290.0
140.00	227.0
141.00	1921.0
142.00	343.0
143.00	2423.0
144.00	138.0
145.10	442.0
146.00	280.0
147.00	143.0
148.00	399.0
148.90	100.0
149.90	173.0
154.10	180.0
155.10	454.0
156.90	164.0
159.00	206.0
161.00	236.0
170.00	160.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

172.00	1165.0
174.10	113632.0
175.10	8915.0
176.10	108304.0
177.10	6625.0
178.20	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	2286.0
37.00	12268.0
38.00	11386.0
39.00	4756.0
40.00	280.0
40.70	127.0
43.00	139.0
44.10	1638.0
45.00	2339.0
46.20	194.0
47.00	2631.0
47.90	1478.0
49.00	9589.0
50.00	43024.0
51.10	12919.0
52.00	652.0
53.00	120.0
55.10	858.0
56.10	4273.0
57.00	6662.0
58.00	227.0
60.10	2218.0
61.00	11396.0
62.00	11256.0
63.00	8160.0
64.00	942.0
65.00	1216.0
66.10	132.0
67.20	432.0
68.00	21592.0
69.10	20536.0
70.00	1773.0
71.10	113.0
72.10	1162.0
73.10	10298.0
74.10	38760.0
75.10	111944.0
76.10	8636.0
77.00	1066.0
79.00	10762.0
80.00	2902.0
81.00	11092.0
82.00	2371.0
83.00	369.0
86.00	213.0
87.10	8050.0
88.00	6665.0
90.90	1176.0
92.10	6160.0
93.10	9485.0
94.10	25424.0
95.10	192320.0
96.10	13172.0
97.00	374.0
102.90	143.0
104.00	1247.0
105.00	297.0
106.00	990.0
106.80	215.0
110.00	180.0
111.00	279.0
111.90	177.0
113.00	244.0
114.90	259.0
116.00	958.0
117.00	1329.0
117.90	1074.0
119.00	1643.0
123.90	199.0
125.80	107.0
128.00	680.0
128.90	348.0
130.00	926.0
130.90	244.0
134.90	342.0
137.00	398.0
139.90	255.0
141.00	2140.0
141.90	361.0
143.00	2589.0
144.00	158.0
145.10	410.0
146.00	297.0
147.00	102.0
148.00	486.0
149.80	173.0
154.10	142.0
155.10	498.0
156.90	263.0
159.10	204.0
161.00	207.0
170.00	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

171.10	201.0
172.00	1125.0
174.10	129264.0
175.10	9947.0
176.10	124720.0
177.10	7622.0
178.10	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	2238.0
37.00	11911.0
38.00	11104.0
39.00	4640.0
40.00	235.0
43.00	143.0
44.00	1656.0
45.00	2252.0
46.10	228.0
47.00	2565.0
47.90	1495.0
49.00	9357.0
50.00	42944.0
51.00	12906.0
52.00	658.0
55.10	712.0
56.10	4203.0
57.10	6393.0
58.10	216.0
60.00	2099.0
61.00	11229.0
62.00	10936.0
63.00	7992.0
64.00	972.0
65.00	1055.0
68.00	22048.0
69.10	21488.0
70.00	1869.0
71.10	168.0
72.10	1254.0
73.10	10471.0
74.10	39120.0
75.10	112200.0
76.00	8654.0
77.10	999.0
79.00	10461.0
80.00	2863.0
81.00	11094.0
82.00	2316.0
83.00	325.0
85.90	202.0
87.00	7931.0
88.00	6705.0
90.90	1262.0
92.10	6363.0
93.10	8999.0
94.10	25192.0
95.10	192320.0
96.10	12932.0
97.00	388.0
102.80	147.0
104.00	1276.0
105.00	331.0
106.00	1026.0
106.70	240.0
107.20	148.0
109.90	170.0
111.00	291.0
111.80	228.0
112.80	207.0
114.90	249.0
116.00	980.0
117.00	1336.0
118.00	937.0
119.00	1520.0
123.90	185.0
125.90	138.0
128.00	664.0
128.90	374.0
130.00	815.0
130.90	241.0
135.00	459.0
137.00	494.0
139.90	238.0
141.00	2315.0
141.90	338.0
143.00	2726.0
144.00	137.0
144.80	416.0
146.00	320.0
148.00	505.0
149.80	140.0
150.20	116.0
152.00	107.0
155.00	529.0
156.90	296.0
158.70	126.0
159.10	170.0
161.00	214.0
171.20	263.0
172.00	1022.0
174.10	133888.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

175.10	9995.0
176.10	129000.0
177.10	8076.0
178.00	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

Scan 2874 (10.581 min): VU040141.D
BFB02

m/z	Abundance
40.00	102.0
43.80	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02