

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
Data File : VU044661.D
Acq On : 16 Sep 2021 14:38
Operator : SY/MD
Sample : M3763-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C92

Quant Time: Sep 17 03:01:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 17 02:59:59 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:34:16 PM

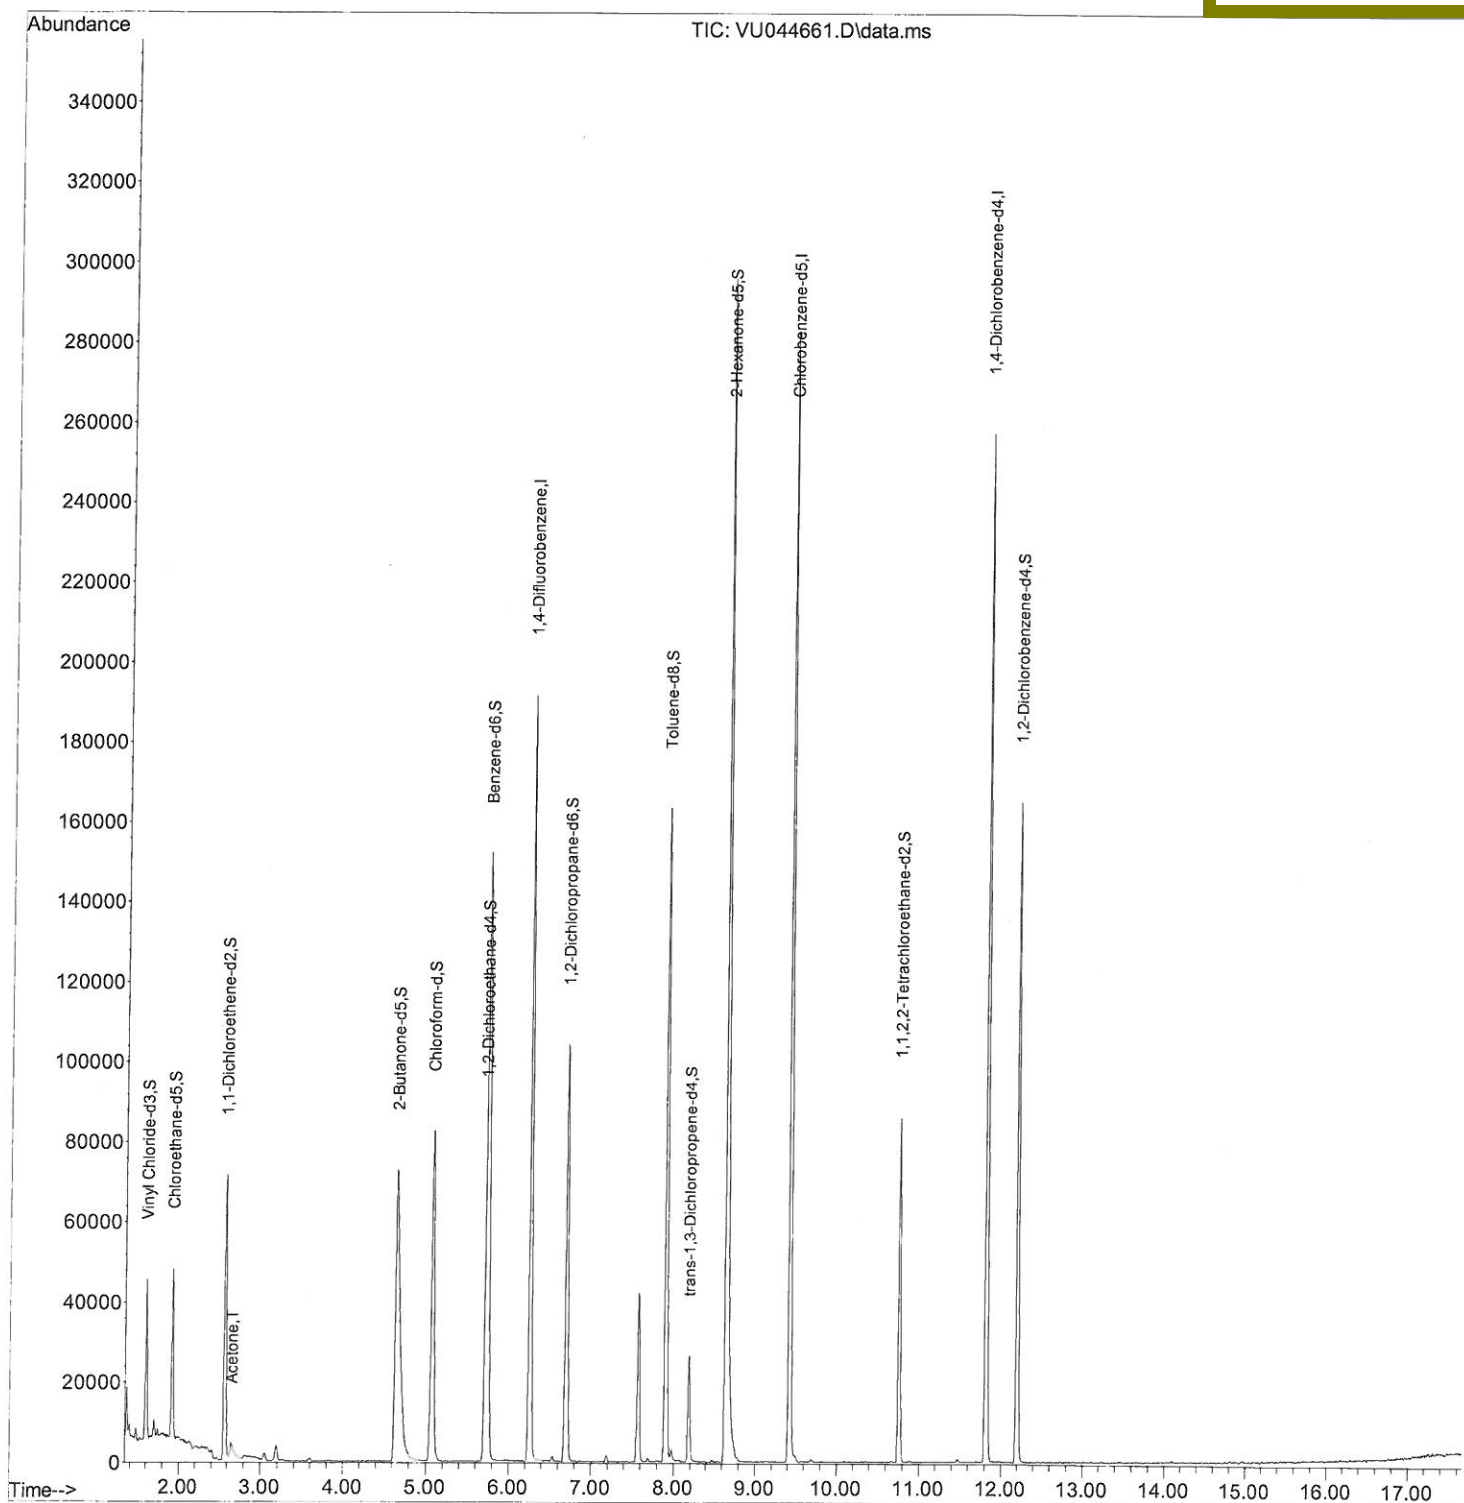

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
 Data File : VU044661.D
 Acq On : 16 Sep 2021 14:38
 Operator : SY/MD
 Sample : M3763-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C92

Quant Time: Sep 17 03:01:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 17 02:59:59 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:34:16 PM

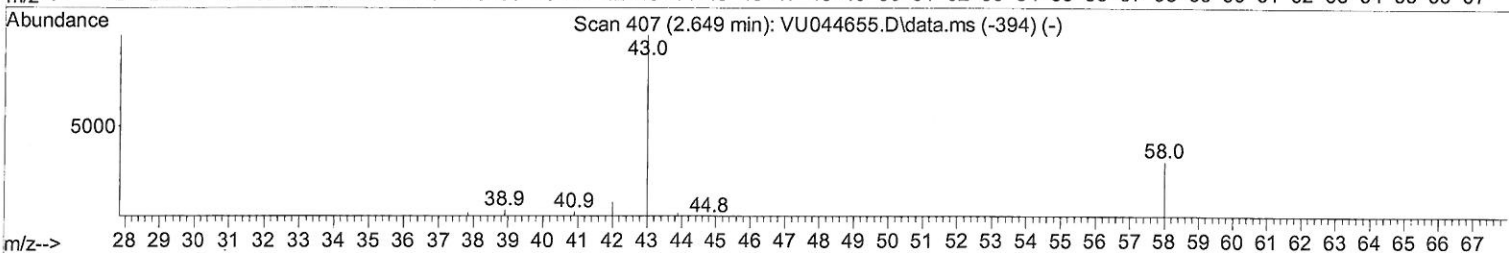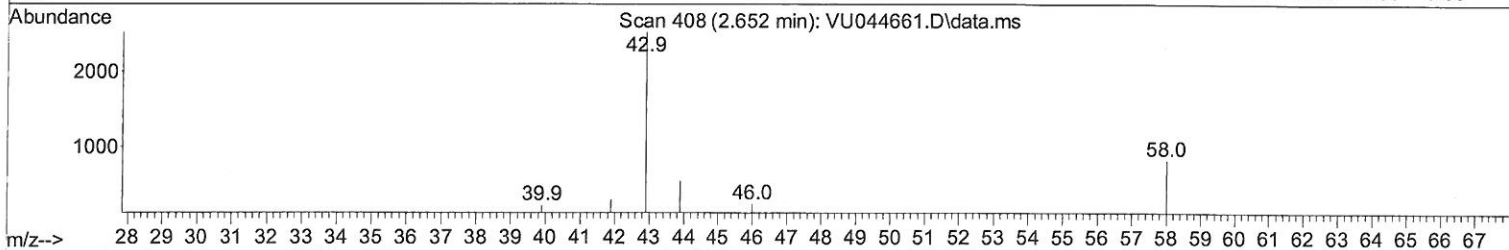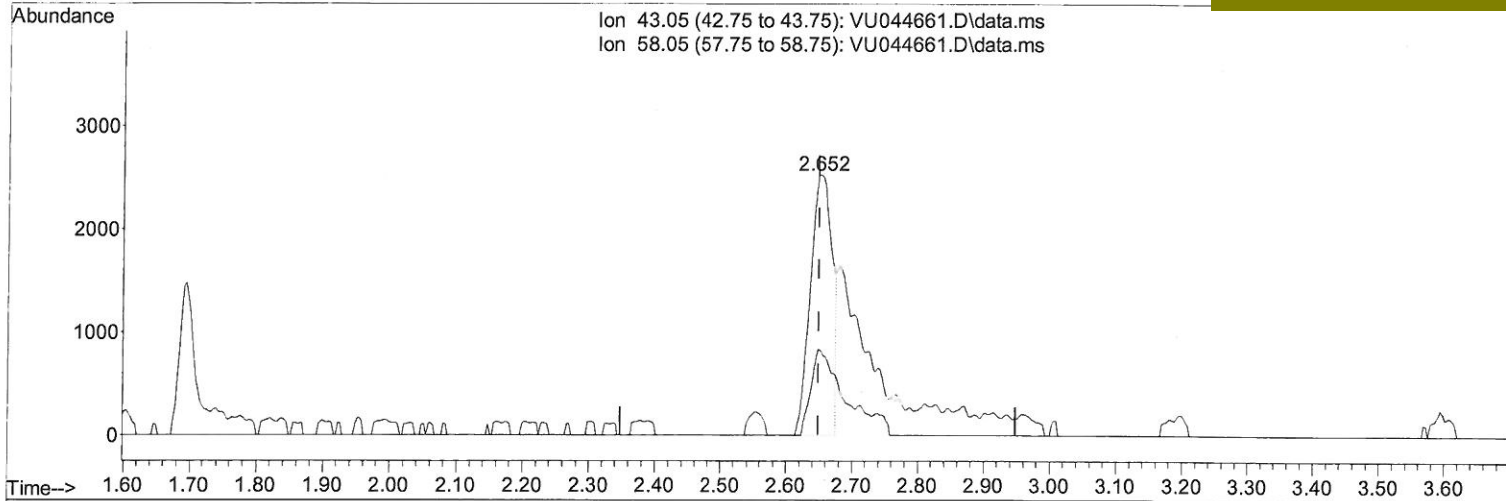

TIC: VU044661.D\data.ms

(13) Acetone (T)

2.652min (+ 0.003) 2.47 ug/L

response 5798

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	21.20	41.24
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
Data File : VU044661.D
Acq On : 16 Sep 2021 14:38
Operator : SY/MD
Sample : M3763-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C92

Quant Time: Sep 17 03:01:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 17 02:59:59 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:34:16 PM

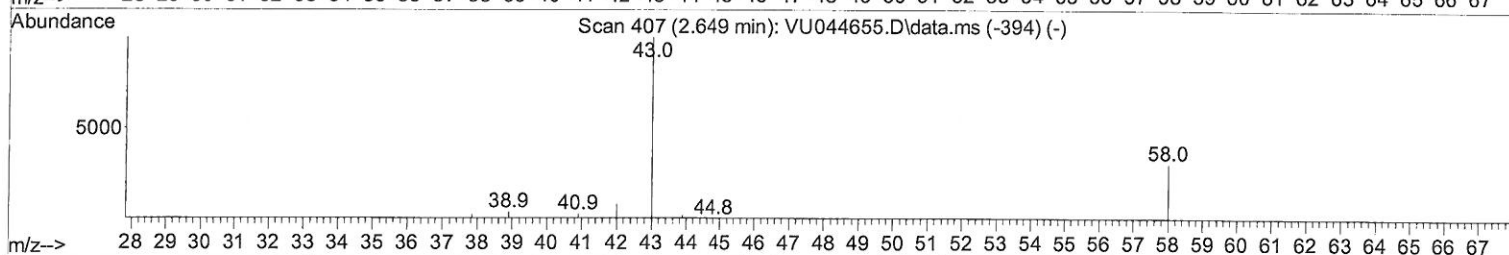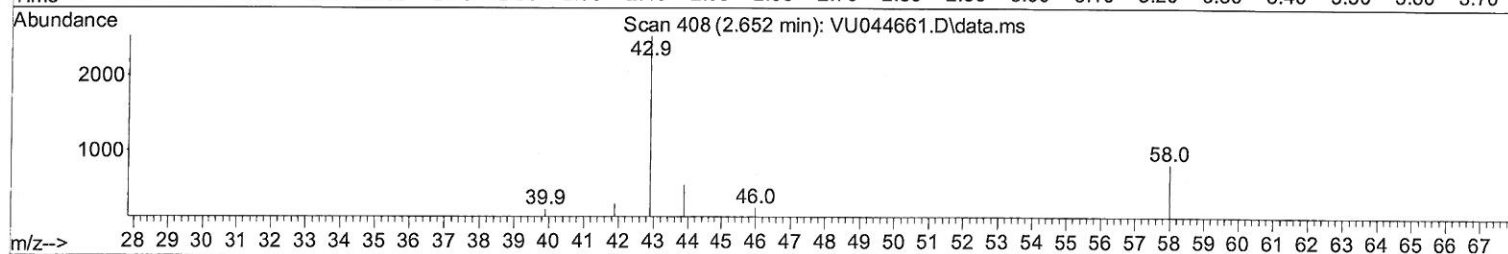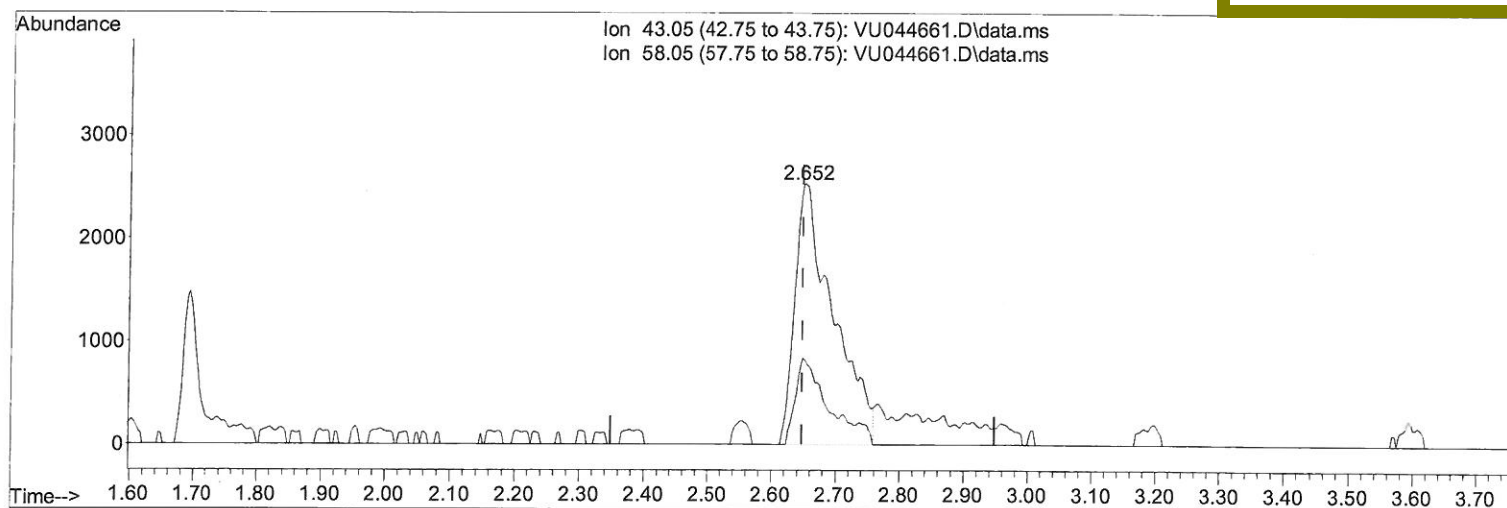

TIC: VU044661.D\data.ms

(13) Acetone (T)

2.652min (+ 0.003) 4.46 ug/L m

response 10482

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	21.20	22.81
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
 Data File : VU044661.D
 Acq On : 16 Sep 2021 14:38
 Operator : SY/MD
 Sample : M3763-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0C92

Quant Time: Sep 17 03:01:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 17 02:59:59 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:34:16 PM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	145730	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	146916	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	62126	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	25965	3.020	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	60.400%		
7) Chloroethane-d5	1.919	69	30281	3.451	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	69.000%		
11) 1,1-Dichloroethene-d2	2.572	65	13953	3.213	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	64.200%		
20) 2-Butanone-d5	4.646	46	162229	45.007	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	90.020%		
24) Chloroform-d	5.070	84	71698	3.964	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	79.200%		
26) 1,2-Dichloroethane-d4	5.710	65	43710	4.053	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	81.000%		
32) Benzene-d6	5.736	84	134298	3.585	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	71.800%		
36) 1,2-Dichloropropane-d6	6.697	67	47911	3.894	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	77.800%		
41) Toluene-d8	7.903	98	103228	3.165	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	63.400%#		
43) trans-1,3-Dichloroprop...	8.186	79	14787	3.410	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	68.200%		
46) 2-Hexanone-d5	8.645	63	118430	42.491	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	84.980%		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	43501	3.988	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	79.800%		
66) 1,2-Dichlorobenzene-d4	12.198	152	40611	3.962	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	79.200%#		

Target Compounds

13) Acetone	2.652	43	10482m	4.465	ug/L	Qvalue
-------------	-------	----	--------	-------	------	--------

MD
09/21/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed