


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
Data File : VU044669.D
Acq On : 16 Sep 2021 18:12
Operator : SY/MD
Sample : M3763-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC0

Quant Time: Sep 17 03:03:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 17 02:59:59 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:34:41 PM

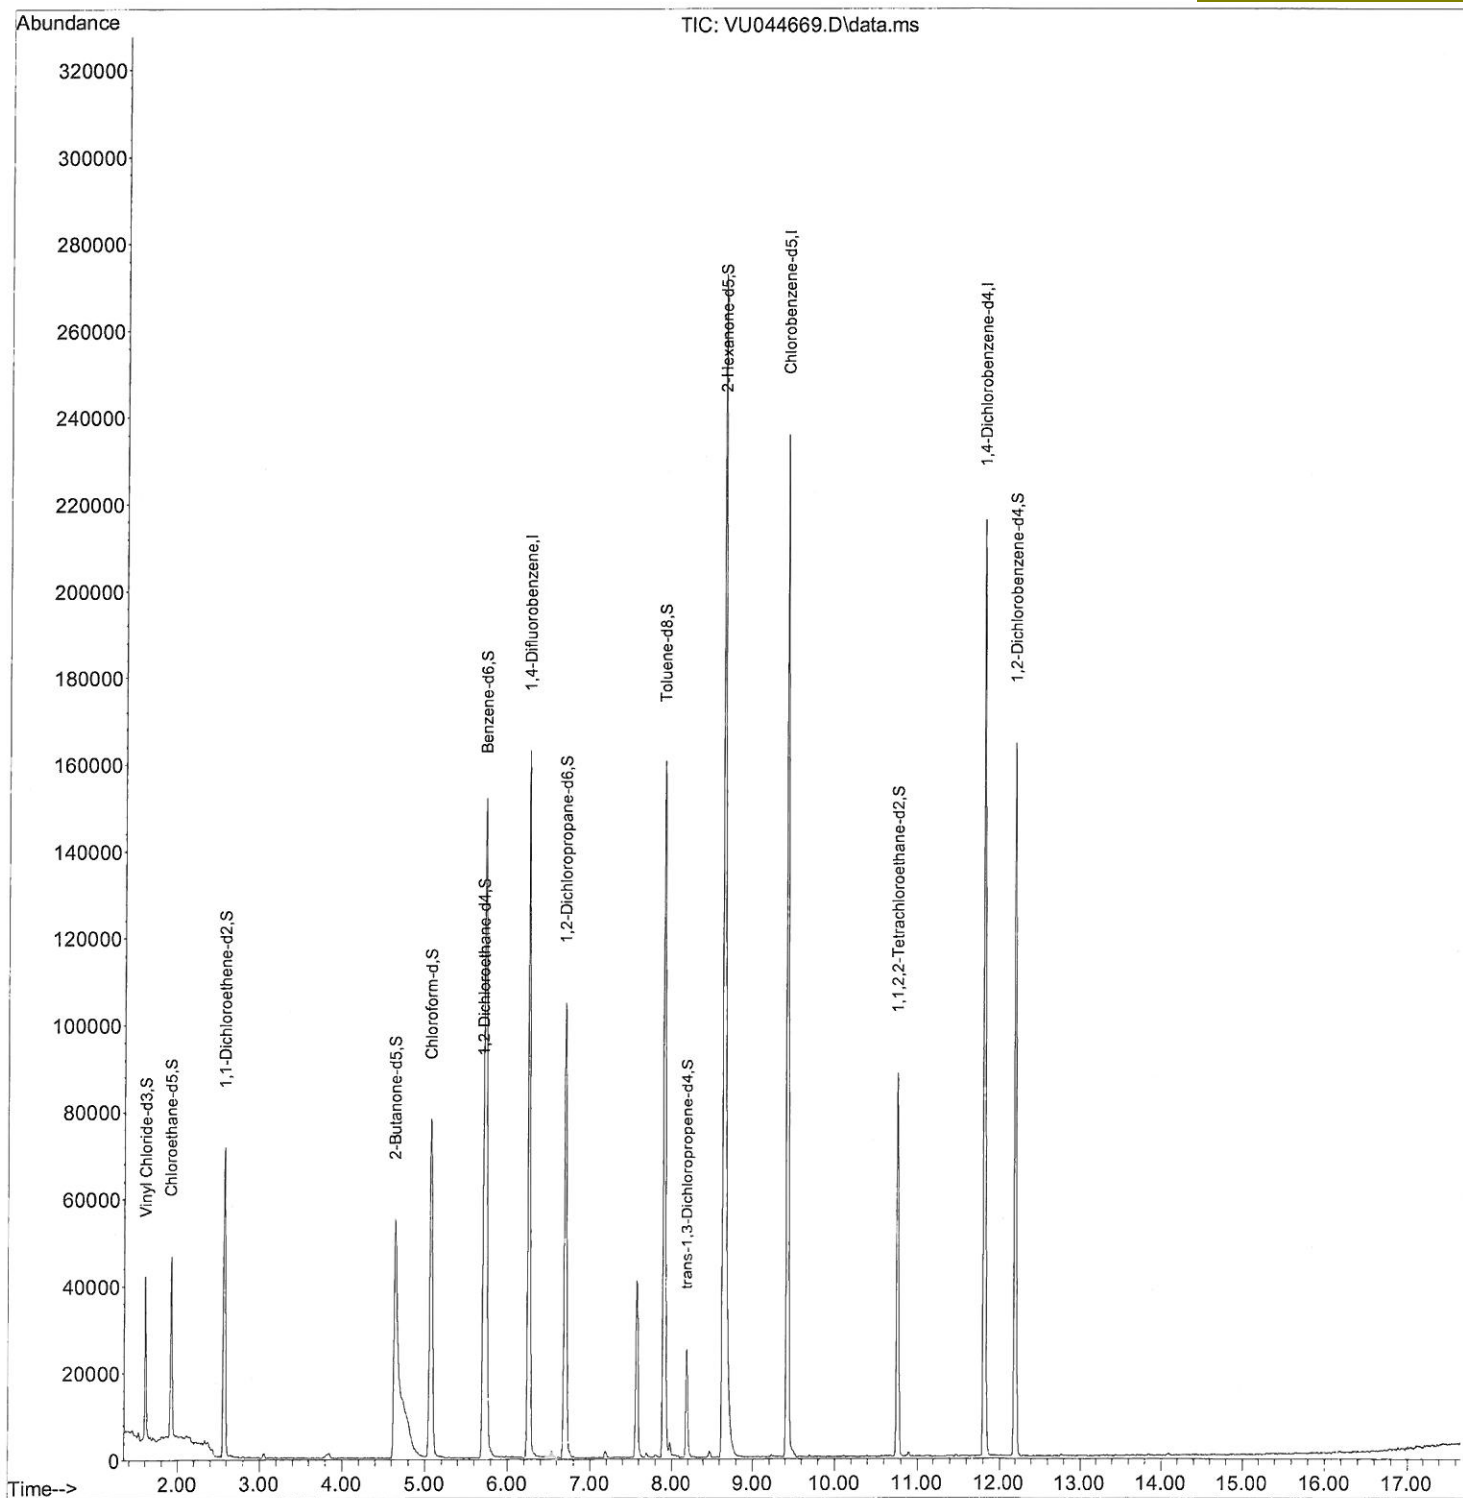

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
 Data File : VU044669.D
 Acq On : 16 Sep 2021 18:12
 Operator : SY/MD
 Sample : M3763-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CC0

Quant Time: Sep 17 03:03:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 17 02:59:59 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:34:41 PM

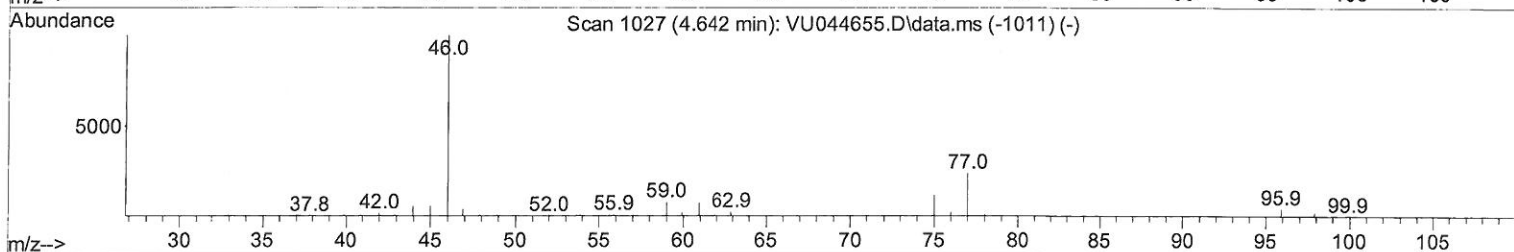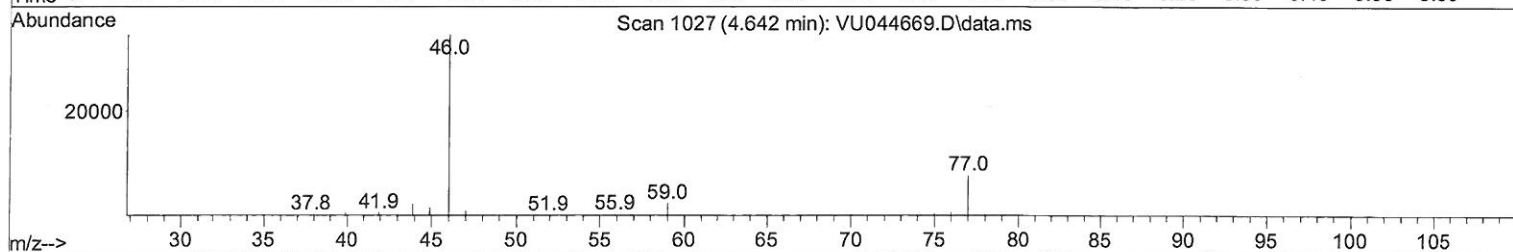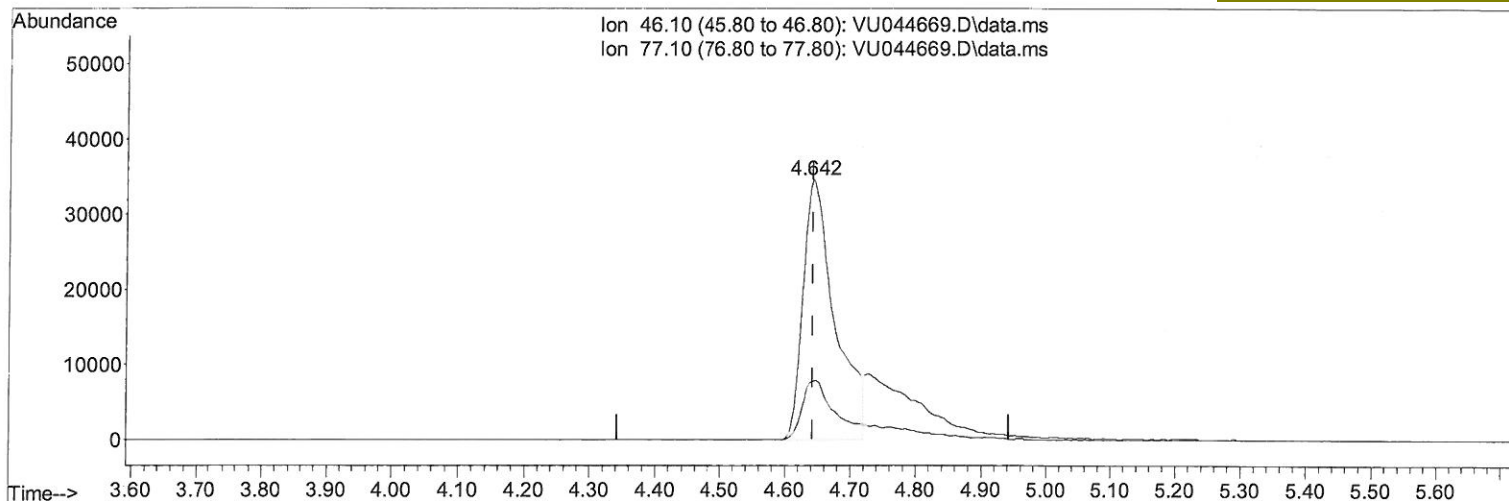

TIC: VU044669.D\data.ms

(20) 2-Butanone-d5 (S)

4.642min (+ 0.000) 38.14 ug/L

response 117791

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.40	22.18
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
Data File : VU044669.D
Acq On : 16 Sep 2021 18:12
Operator : SY/MD
Sample : M3763-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC0

Quant Time: Sep 17 03:03:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 17 02:59:59 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:34:41 PM

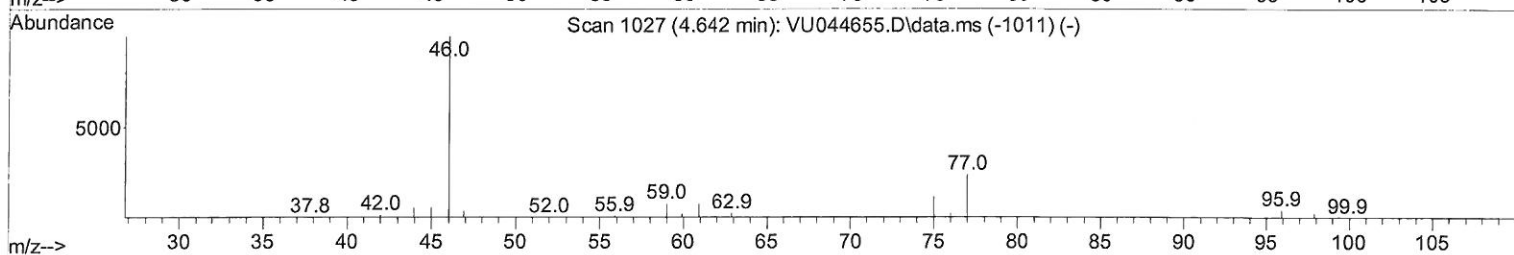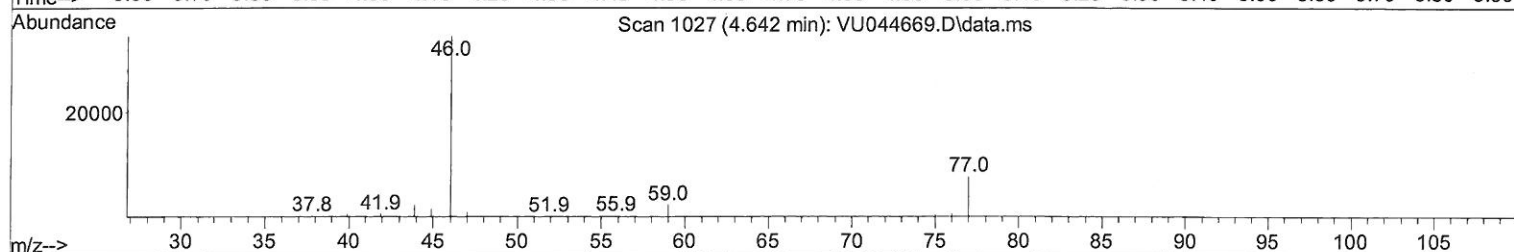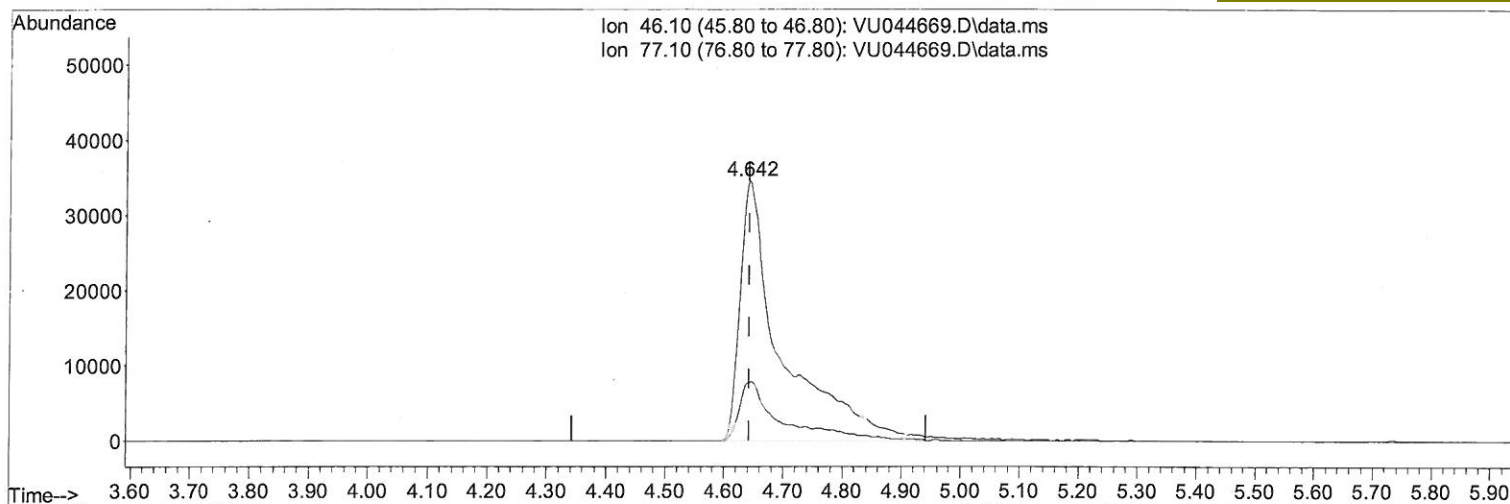

TIC: VU044669.D\data.ms

(20) 2-Butanone-d5 (S)

4.642min (+ 0.000) 54.49 ug/L m

response 168263

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.40	15.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
 Data File : VU044669.D
 Acq On : 16 Sep 2021 18:12
 Operator : SY/MD
 Sample : M3763-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sample ID :
 C0CC0

Quant Time: Sep 17 03:03:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 17 02:59:59 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MM Dadoda
 9/17/2021 4:34:41 PM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	124854	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	124017	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	53229	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	25649	3.482	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery =	69.600%		
7) Chloroethane-d5	1.916	69	30332	4.035	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery =	80.600%		
11) 1,1-Dichloroethene-d2	2.571	65	13927	3.743	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery =	74.800%		
20) 2-Butanone-d5	4.642	46	168263m	54.487	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery =	108.980%		
24) Chloroform-d	5.070	84	70563	4.554	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery =	91.000%		
26) 1,2-Dichloroethane-d4	5.710	65	43689	4.728	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery =	94.600%		
32) Benzene-d6	5.735	84	132796	4.200	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery =	84.000%		
36) 1,2-Dichloropropane-d6	6.697	67	49096	4.728	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery =	94.600%		
41) Toluene-d8	7.902	98	103425	3.757	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery =	75.200%		
43) trans-1,3-Dichloroprop...	8.185	79	14337	3.916	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery =	78.400%		
46) 2-Hexanone-d5	8.645	63	124272	52.820	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery =	105.640%		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44337	4.815	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery =	96.400%		
66) 1,2-Dichlorobenzene-d4	12.198	152	39811	4.533	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery =	90.600%		

7 MB
 09/21/21

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed