

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
 Data File : VU044661.D
 Acq On : 16 Sep 2021 14:38
 Operator : SY/MD
 Sample : M3763-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C92

Manual Integrations
 APPROVED

MMDadoda
 9/17/2021 4:34:16 PM

Quant Time: Sep 17 03:01:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 17 02:59:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	145730	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	146916	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	62126	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	25965	3.020	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	60.400%
7) Chloroethane-d5	1.919	69	30281	3.451	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.000%
11) 1,1-Dichloroethene-d2	2.572	65	13953	3.213	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.200%
20) 2-Butanone-d5	4.646	46	162229	45.007	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.020%
24) Chloroform-d	5.070	84	71698	3.964	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.200%
26) 1,2-Dichloroethane-d4	5.710	65	43710	4.053	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
32) Benzene-d6	5.736	84	134298	3.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	71.800%
36) 1,2-Dichloropropane-d6	6.697	67	47911	3.894	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	77.800%
41) Toluene-d8	7.903	98	103228	3.165	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.400%#
43) trans-1,3-Dichloroprop...	8.186	79	14787	3.410	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.200%
46) 2-Hexanone-d5	8.645	63	118430	42.491	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.980%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	43501	3.988	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	40611	3.962	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.200%#
Target Compounds						Qvalue
13) Acetone	2.652	43	10482m	4.465	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
Data File : VU044661.D
Acq On : 16 Sep 2021 14:38
Operator : SY/MD
Sample : M3763-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0C92

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:34:16 PM




Quant Time: Sep 17 03:01:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 17 02:59:59 2021
Response via : Initial Calibration

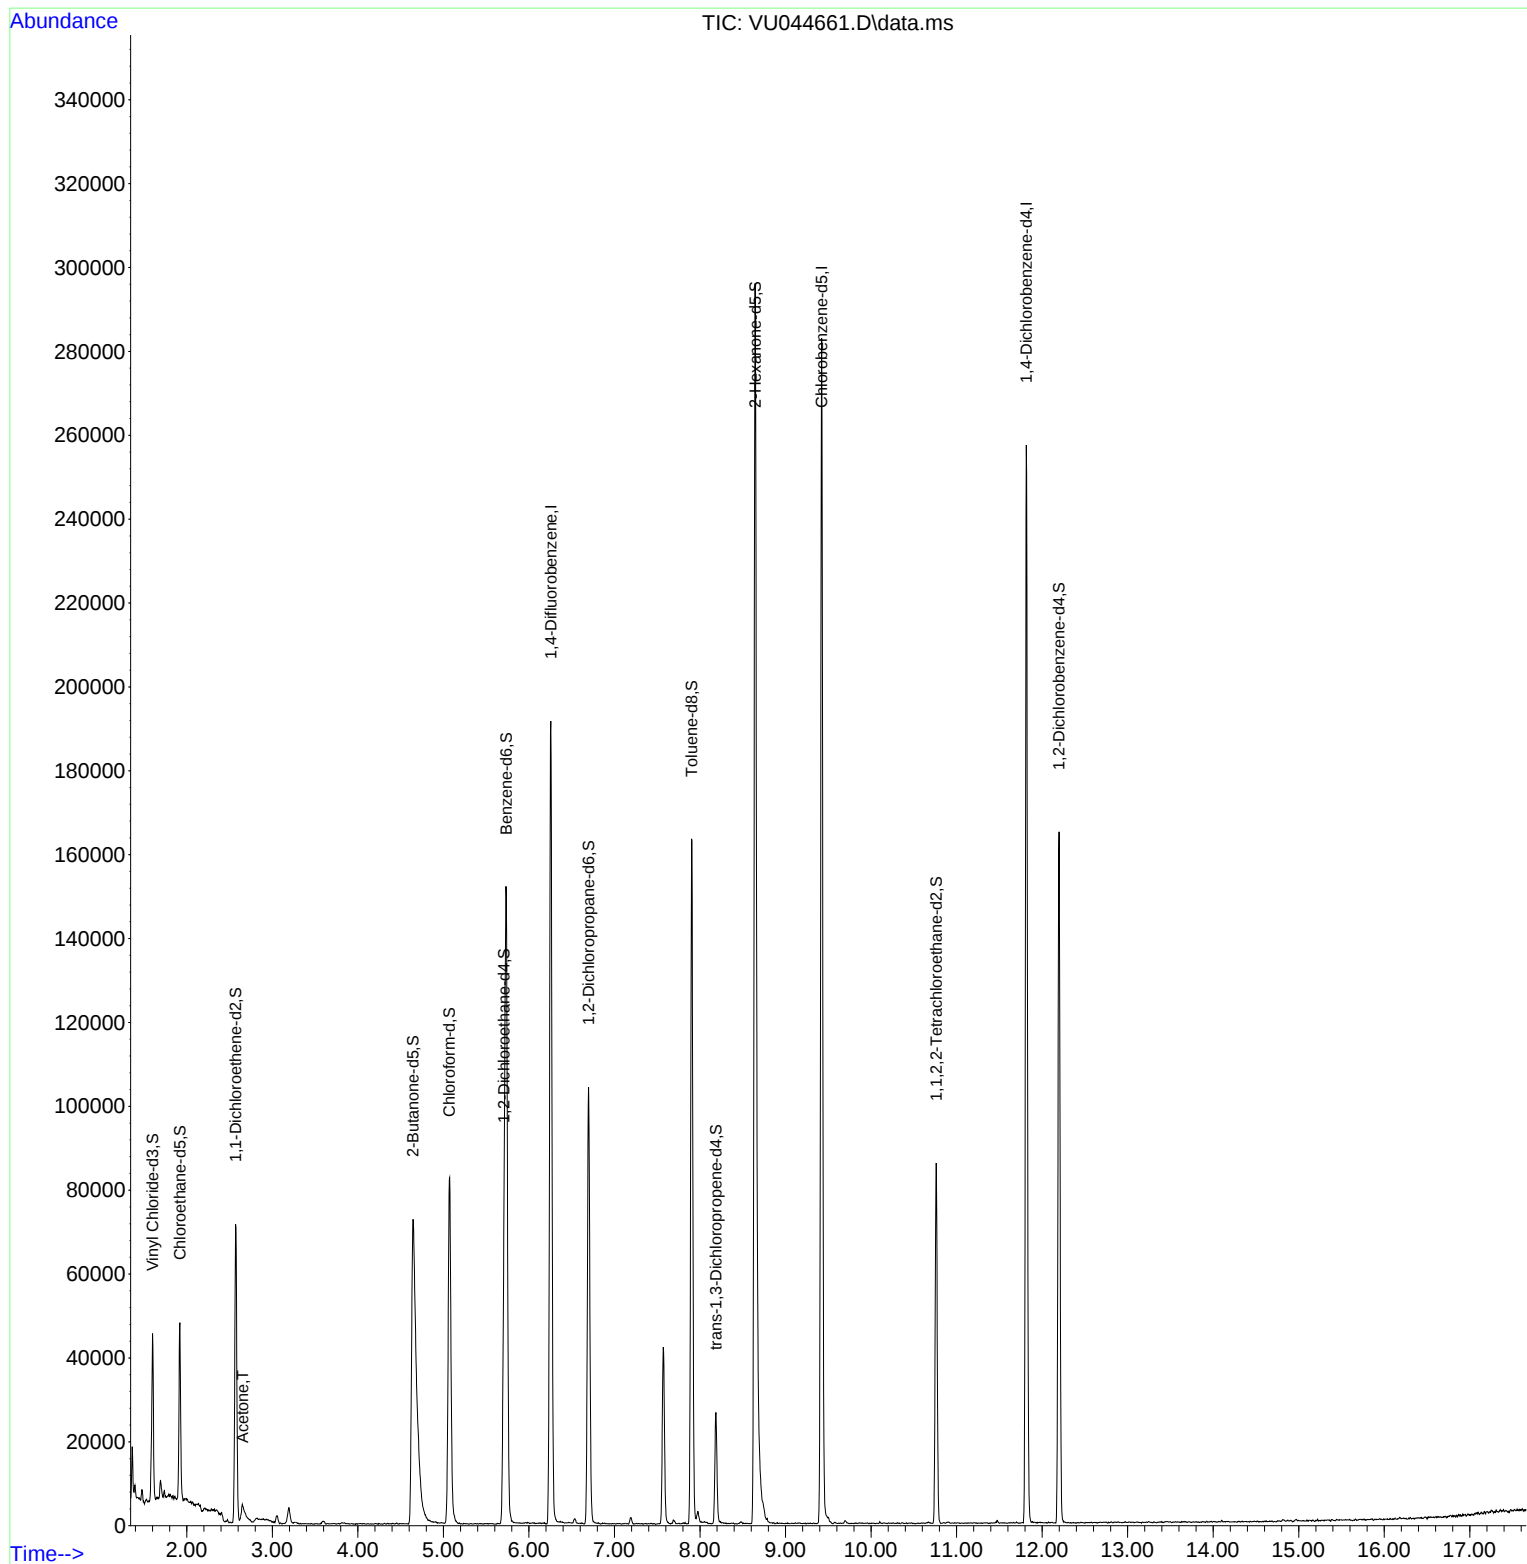

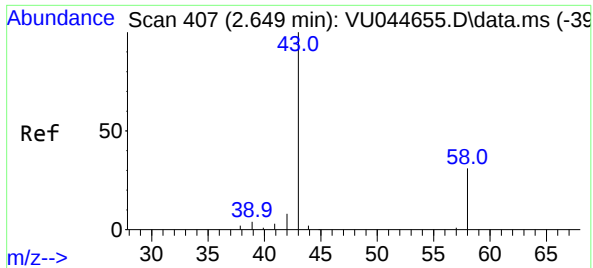

#13
Acetone
Concen: 4.465 ug/L m
RT: 2.652 min Scan# 408
Delta R.T. 0.003 min
Lab File: VU044661.D
Acq: 16 Sep 2021 14:38

Tgt Ion: 43 Resp: 10482
Ion Ratio Lower Upper
43 100
58 22.8 0.0 42.4

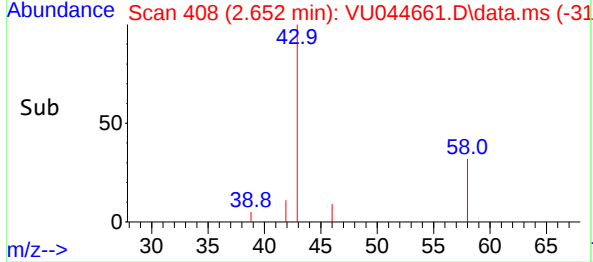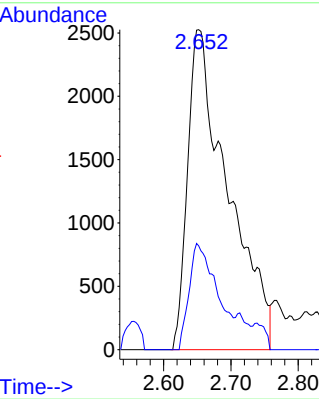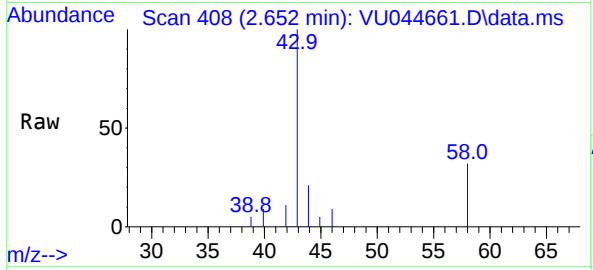

Instrument :
MSVOA_U
ClientSampleId :
C0C92

Manual Integrations
APPROVED

MMDadoda
9/17/2021 4:34:16 PM