


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091621\
Data File : VU044654.D
Acq On : 16 Sep 2021 09:25
Operator : SY/MD
Sample : BFB019
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB019

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 18 01:28:45 2021

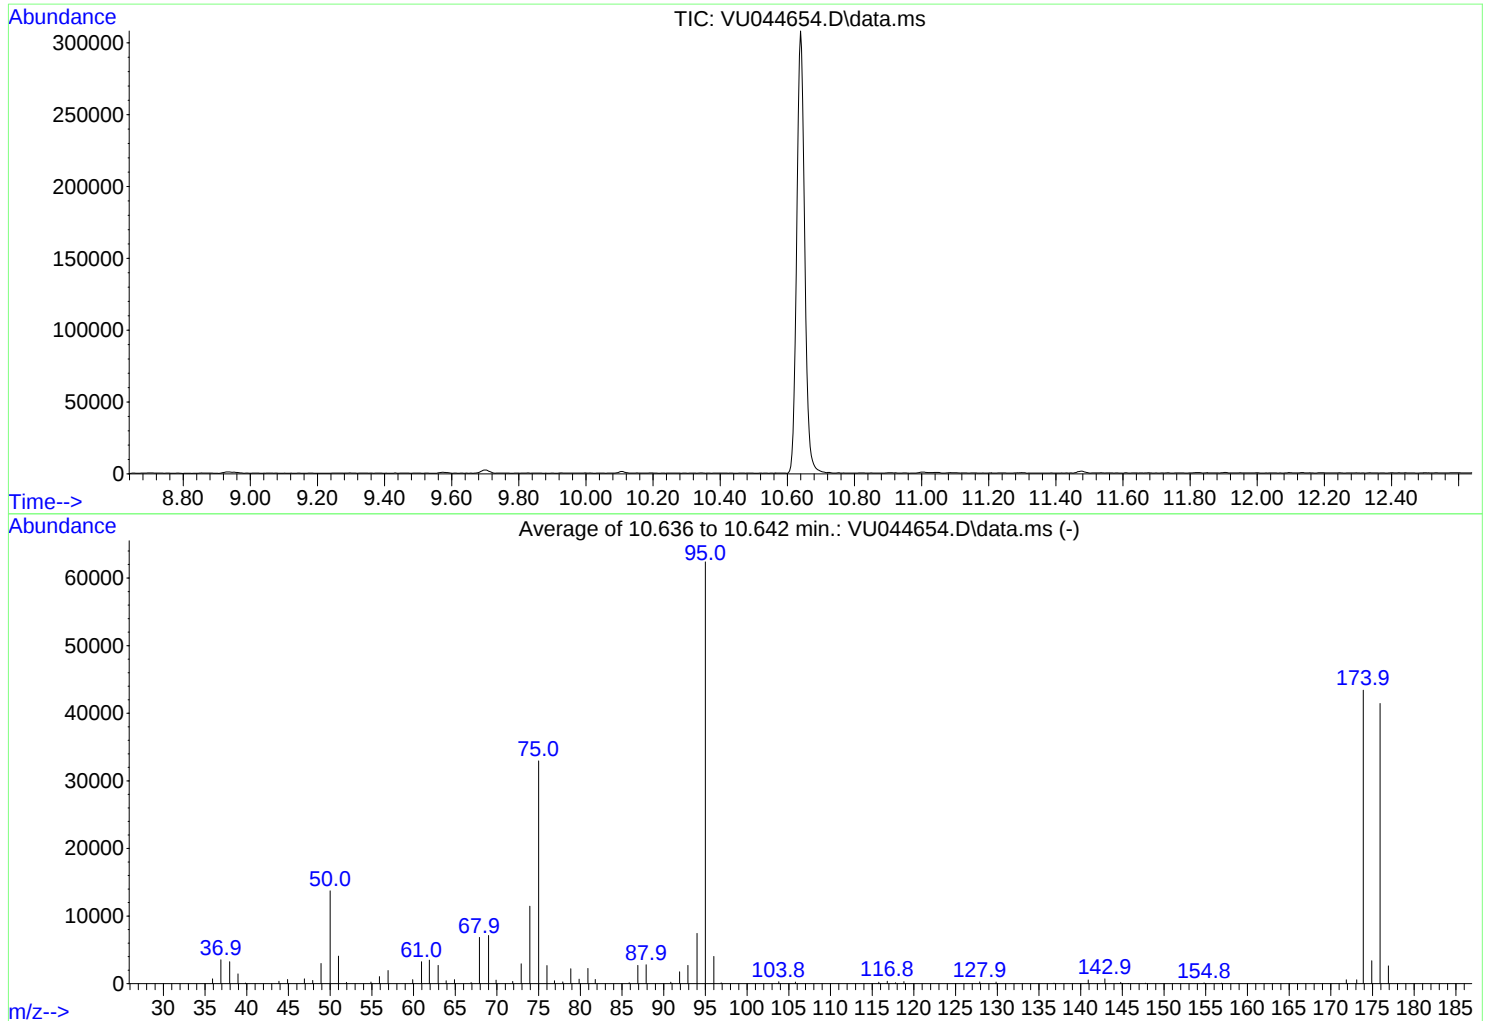

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.0	13732	PASS
75	95	30	80	52.8	32949	PASS
95	95	100	100	100.0	62395	PASS
96	95	5	9	6.4	4015	PASS
173	174	0.00	2	1.3	573	PASS
174	95	50	120	69.6	43405	PASS
175	174	5	9	7.8	3388	PASS
176	174	95	101	95.5	41451	PASS
177	176	5	9	6.3	2624	PASS

m/z	Abundance
35.90	740.0
36.90	3339.0
37.90	3186.0
38.90	1386.0
39.90	254.0
43.90	717.0
44.90	594.0
46.90	691.0
47.90	438.0
48.90	2893.0
50.00	13361.0
51.00	3922.0
52.00	156.0
54.90	212.0
55.90	982.0
57.00	1970.0
59.90	616.0
60.90	3264.0
61.90	3338.0
62.90	2652.0
63.90	426.0
64.90	587.0
66.90	168.0
67.90	6645.0
69.00	6943.0
69.90	511.0
71.90	306.0
72.90	2927.0
74.00	11538.0
75.00	32312.0
76.00	2651.0
76.90	439.0
77.90	277.0
78.90	2181.0
79.80	635.0
80.90	2215.0
81.80	637.0
85.80	117.0
86.90	2717.0
87.90	2744.0
90.80	230.0
91.90	1661.0
92.90	2674.0
94.00	7334.0
95.00	61368.0
96.00	3900.0
96.90	131.0
103.80	265.0
105.80	238.0
115.80	181.0
116.80	378.0
117.80	176.0
118.80	346.0
127.90	252.0
129.90	243.0
140.90	582.0
142.90	759.0
144.80	172.0
147.80	135.0
154.80	128.0
156.90	106.0
158.90	100.0
171.80	559.0
173.10	608.0
173.90	44160.0
174.90	3295.0
175.90	41992.0
176.90	2573.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
39.90	151.0
43.80	394.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	668.0
36.90	3610.0
38.00	3223.0
39.00	1473.0
39.80	242.0
43.90	760.0
44.90	621.0
46.90	721.0
47.90	520.0
48.90	2952.0
50.00	13746.0
51.00	4135.0
51.90	230.0
54.90	251.0
55.90	1039.0
56.90	1859.0
59.90	576.0
60.90	3181.0
61.90	3501.0
63.00	2631.0
63.90	407.0
64.90	575.0
66.90	165.0
67.90	6823.0
69.00	7033.0
69.90	526.0
71.90	340.0
72.90	2825.0
73.90	11039.0
75.00	32624.0
76.00	2621.0
76.90	399.0
77.90	219.0
78.80	2152.0
79.90	663.0
80.90	2202.0
81.80	549.0
85.90	146.0
86.90	2594.0
87.90	2738.0
90.90	212.0
91.90	1806.0
92.90	2672.0
94.00	7320.0
95.00	61280.0
96.00	4011.0
96.90	119.0
103.80	304.0
105.80	211.0
115.80	212.0
116.80	339.0
117.80	137.0
118.80	281.0
127.90	237.0
129.80	233.0
136.80	105.0
140.90	488.0
142.90	633.0
144.80	185.0
154.80	108.0
171.90	562.0
173.10	508.0
173.90	41136.0
174.90	3350.0
175.90	39432.0
176.90	2595.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019

m/z	Abundance
35.90	731.0
36.90	3652.0
38.00	3323.0
39.00	1486.0
39.80	253.0
43.90	749.0
44.90	607.0
46.90	695.0
47.90	493.0
48.90	3096.0
50.00	14090.0
51.00	4193.0
51.90	200.0
54.90	254.0
55.90	1077.0
57.00	2010.0
59.90	584.0
61.00	3301.0
61.90	3612.0
63.00	2786.0
63.90	450.0
64.90	591.0
66.90	171.0
67.90	7043.0
69.00	7372.0
69.90	506.0
71.90	338.0
72.90	3032.0
74.00	11762.0
75.00	33912.0
76.00	2743.0
76.90	428.0
77.90	264.0
78.80	2255.0
79.80	674.0
80.90	2335.0
81.80	632.0
85.80	134.0
86.90	2808.0
87.90	2876.0
90.80	218.0
91.90	1817.0
92.90	2772.0
94.00	7669.0
95.00	64536.0
96.00	4135.0
96.90	136.0
103.80	279.0
105.80	233.0
115.80	212.0
116.80	367.0
117.80	152.0
118.80	331.0
127.90	266.0
129.80	243.0
136.80	106.0
140.90	574.0
142.90	758.0
144.80	210.0
145.70	104.0
147.80	103.0
154.80	126.0
156.90	105.0
171.90	586.0
173.10	602.0
173.90	44920.0
174.90	3519.0
175.90	42928.0
176.90	2704.0

Instrument :
MSVOA_U
ClientSampleId :
BFB019