

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
 Data File : VU050722.D
 Acq On : 16 Sep 2022 13:07
 Operator : JC/MD
 Sample : VU0916WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0916WBL01

Quant Time: Sep 17 01:05:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Aug 25 14:01:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.115	96	43768	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	11975	0.804	ug/l	0.00
Spiked Amount 1.000			Recovery	=	80.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	13845	0.786	ug/l	0.00
Spiked Amount 1.000			Recovery	=	79.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
Data File : VU050722.D
Acq On : 16 Sep 2022 13:07
Operator : JC/MD
Sample : VU0916WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0916WBL01

Quant Time: Sep 17 01:05:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Aug 25 14:01:59 2022
Response via : Initial Calibration




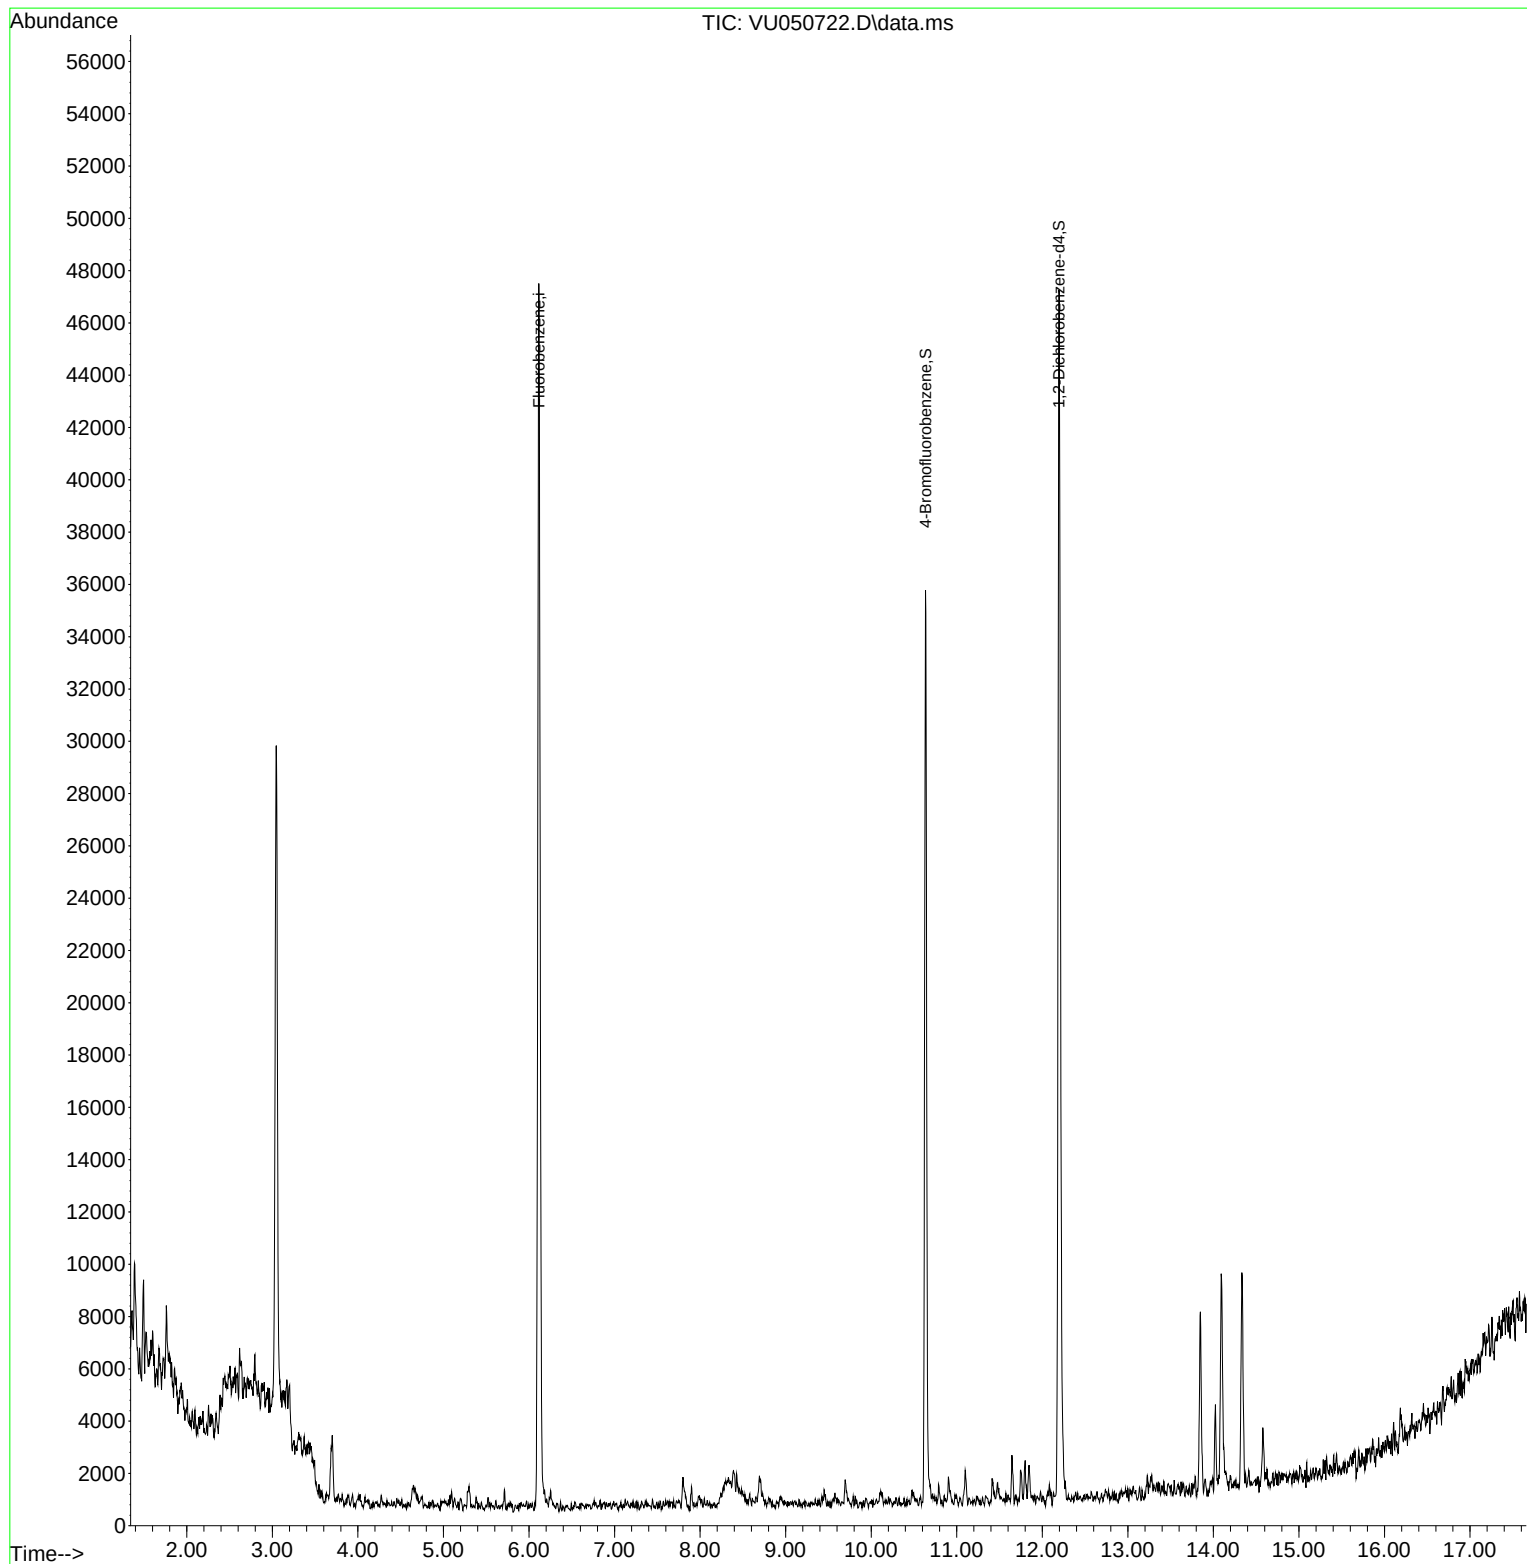


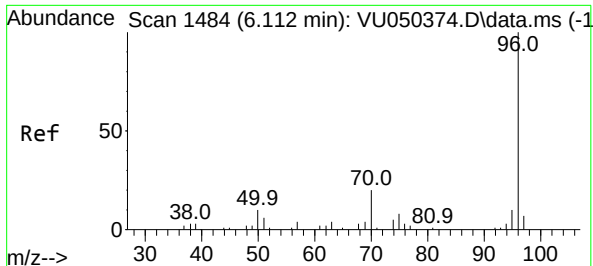

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1484
Delta R.T. -0.000 min
Lab File: VU050722.D
Acq: 16 Sep 2022 13:07




Instrument :
MSVOA_U
ClientSampleId :
VU0916WBL01


Tgt Ion: 96	Resp: 43768
Ion Ratio	Lower Upper
96 100	
70 20.9	16.7 25.1
95 9.1	7.4 11.0
97 6.4	0.0 0.0#

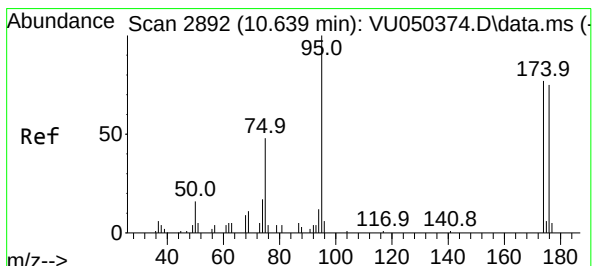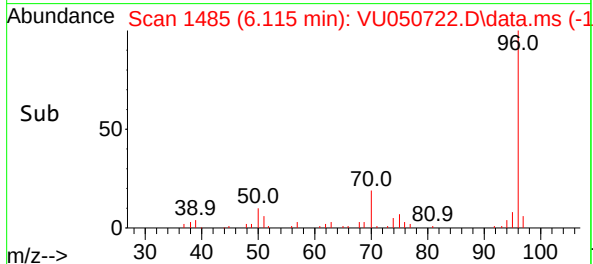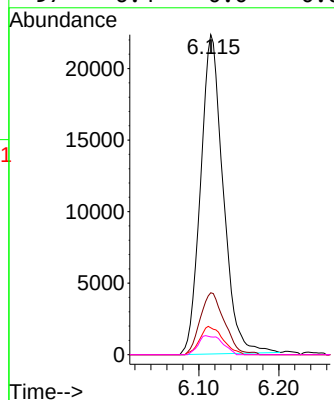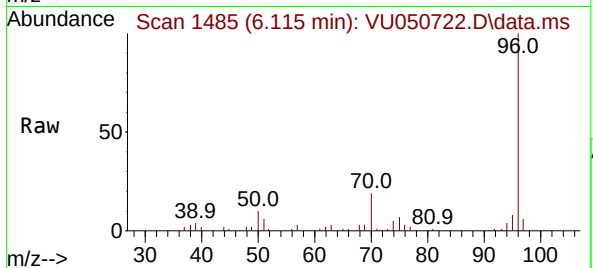

#57
4-Bromofluorobenzene
Concen: 0.804 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU050722.D
Acq: 16 Sep 2022 13:07

Tgt Ion: 95	Resp: 11975
Ion Ratio	Lower Upper
95 100	
174 87.9	62.4 93.6
176 78.2	56.2 84.2

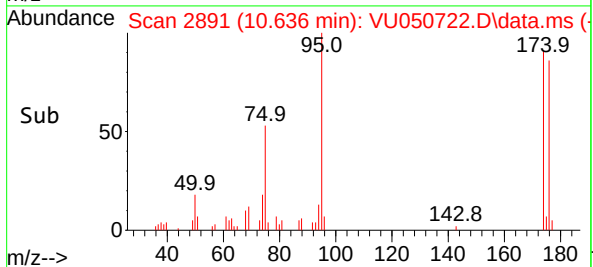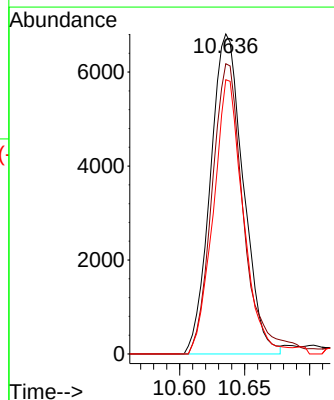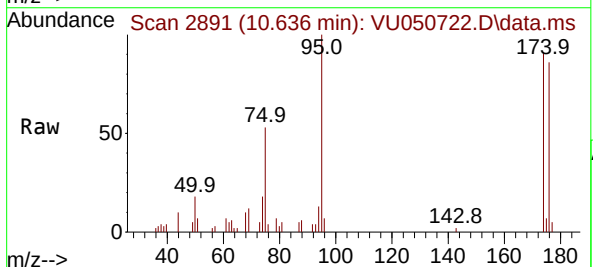

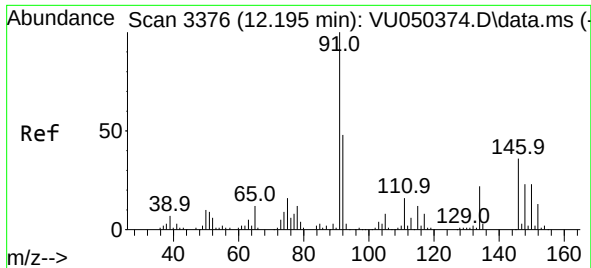

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.786 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VU050722.D
 Acq: 16 Sep 2022 13:07

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0916WBL01

Tgt Ion	Ratio	Lower	Upper
152	100		
115	68.7	0.0	254.6
150	157.1	0.0	623.6

