

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
 Data File : VU050722.D
 Acq On : 16 Sep 2022 13:07
 Operator : JC/MD
 Sample : VU0916WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0916WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU050722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.253	281	284	290	rBV4	1167	1199	1.32%	0.329%
2	2.617	394	397	402	rBV5	1881	2030	2.23%	0.558%
3	3.047	519	531	547	rVB3	25014	47243	51.96%	12.978%
4	3.700	721	734	743	rVB6	2514	4851	5.33%	1.333%
5	6.115	1473	1485	1504	rBV	46741	90930	100.00%	24.979%
6	7.800	2002	2009	2014	rBV4	1193	1632	1.79%	0.448%
7	7.899	2034	2040	2046	rBV	937	1156	1.27%	0.318%
8	8.391	2186	2193	2201	rVB4	804	1418	1.56%	0.390%
9	8.694	2279	2287	2290	rBV3	1010	1292	1.42%	0.355%
10	9.697	2594	2599	2603	rBV2	906	1041	1.14%	0.286%
11	10.636	2881	2891	2907	rBV	34883	56272	61.88%	15.458%
12	10.787	2932	2938	2947	rVB3	760	933	1.03%	0.256%
13	10.902	2967	2974	2979	rBV4	970	1098	1.21%	0.302%
14	11.099	3025	3035	3044	rBV7	1369	2275	2.50%	0.625%
15	11.414	3129	3133	3145	rBV3	891	1328	1.46%	0.365%
16	11.645	3199	3205	3213	rVB4	1869	2325	2.56%	0.639%
17	11.748	3232	3237	3244	rBV3	1170	1585	1.74%	0.435%
18	11.800	3246	3253	3260	rVV4	1503	1891	2.08%	0.519%
19	11.845	3260	3267	3275	rBV5	1301	1795	1.97%	0.493%
20	12.195	3365	3376	3398	rBV2	46080	90845	99.91%	24.956%
21	13.848	3880	3890	3901	rVV3	7045	11464	12.61%	3.149%
22	13.906	3902	3908	3914	rVB3	645	910	1.00%	0.250%
23	14.024	3938	3945	3951	rBV6	3332	4166	4.58%	1.144%
24	14.092	3958	3966	3974	rBV	7840	12850	14.13%	3.530%
25	14.333	4032	4041	4052	rBV4	8190	13766	15.14%	3.782%
26	14.578	4108	4117	4124	rVV4	2263	3344	3.68%	0.919%
27	16.108	4588	4593	4597	rBV3	1278	1193	1.31%	0.328%
28	16.684	4767	4772	4777	rBV5	1503	1922	2.11%	0.528%
29	16.944	4850	4853	4857	rBV5	1288	1271	1.40%	0.349%




Sum of corrected areas: 364025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
Data File : VU050722.D
Acq On : 16 Sep 2022 13:07
Operator : JC/MD
Sample : VU0916WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0916WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

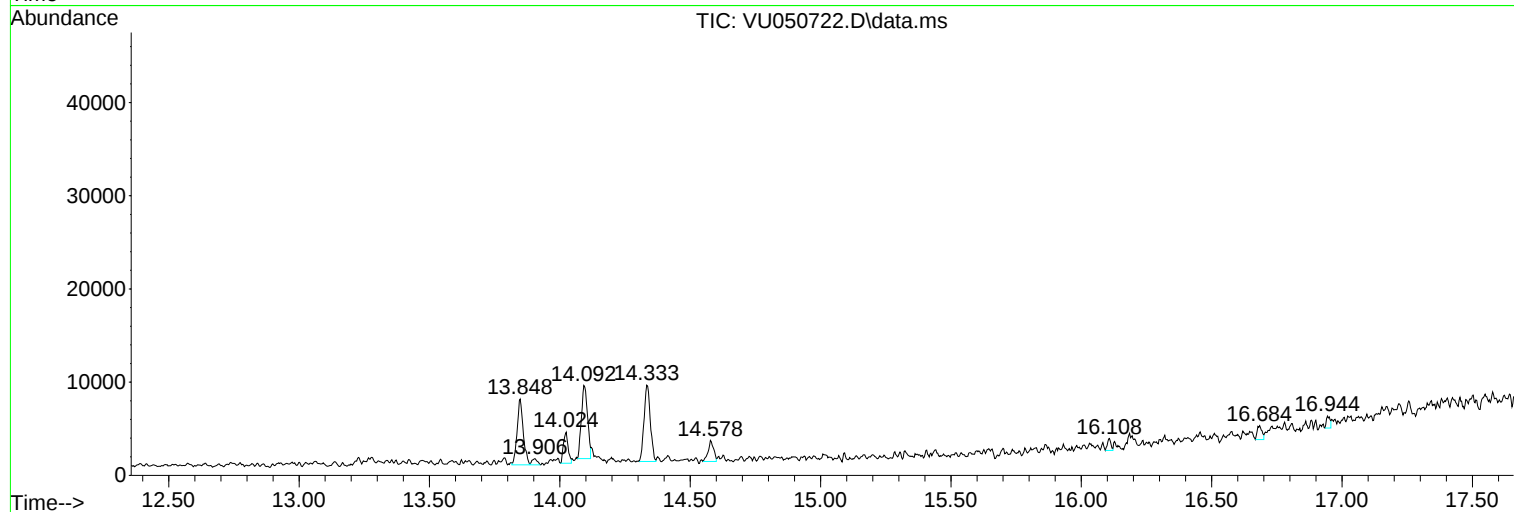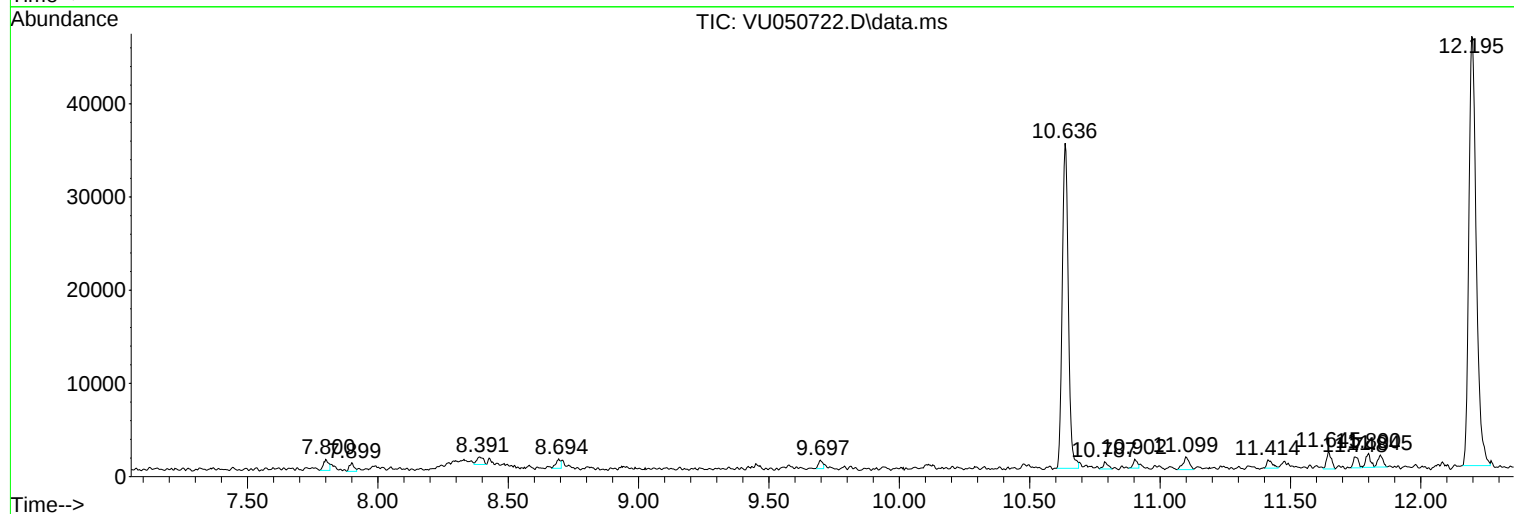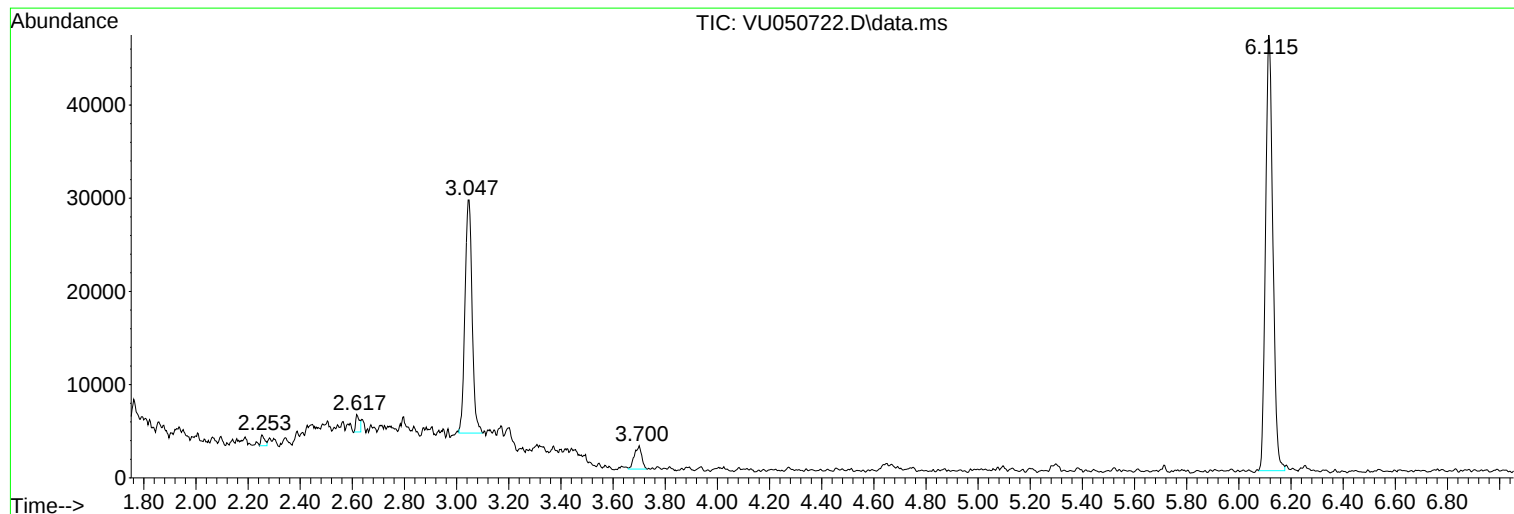

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
Data File : VU050722.D
Acq On : 16 Sep 2022 13:07
Operator : JC/MD
Sample : VU0916WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0916WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
Data File : VU050722.D
Acq On : 16 Sep 2022 13:07
Operator : JC/MD
Sample : VU0916WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0916WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------