

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
 Data File : VU050725.D
 Acq On : 16 Sep 2022 15:02
 Operator : JC/MD
 Sample : N4568-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 38025-110121

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU050725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.044	518	530	548	rVB2	46990	88855	3.07%	1.276%
2	5.089	1148	1166	1191	rBV	1021673	2210602	76.27%	31.757%
3	6.115	1472	1485	1505	rBV	49528	95017	3.28%	1.365%
4	7.105	1778	1793	1826	rBV	1567387	2898263	100.00%	41.636%
5	8.809	2308	2323	2347	rBV	412195	731314	25.23%	10.506%
6	10.292	2768	2784	2802	rBV	448387	766986	26.46%	11.018%
7	10.636	2881	2891	2907	rBV3	38200	62034	2.14%	0.891%
8	12.198	3366	3377	3396	rBV3	51769	107891	3.72%	1.550%




Sum of corrected areas: 6960962

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
Data File : VU050725.D
Acq On : 16 Sep 2022 15:02
Operator : JC/MD
Sample : N4568-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38025-110121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

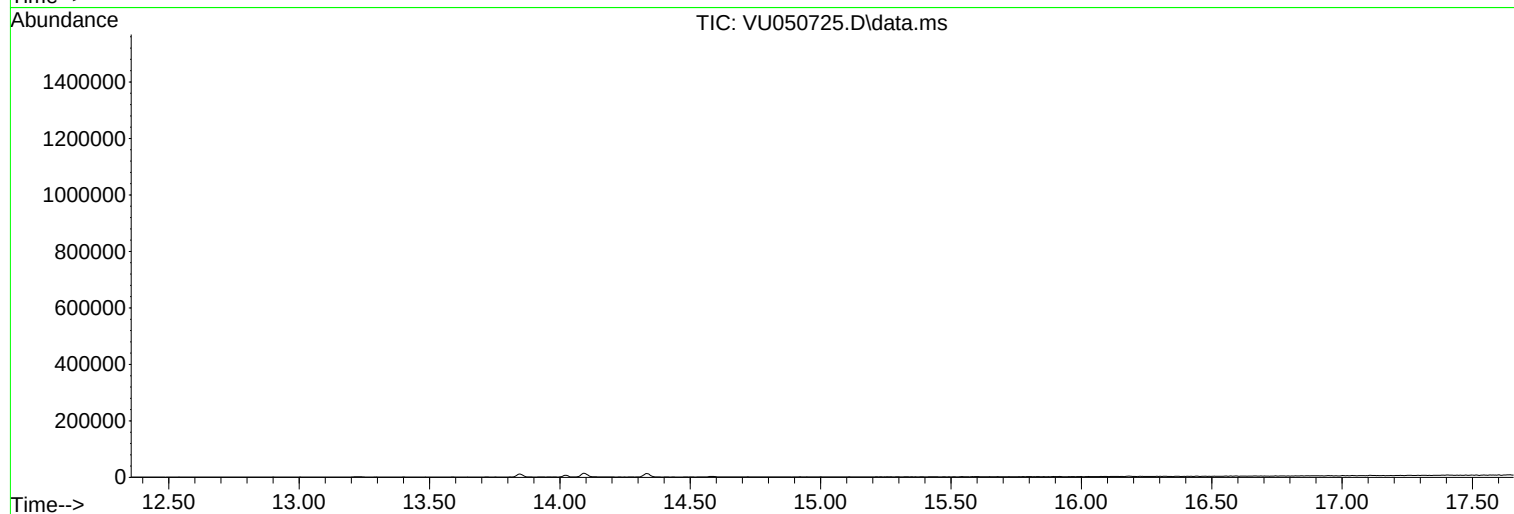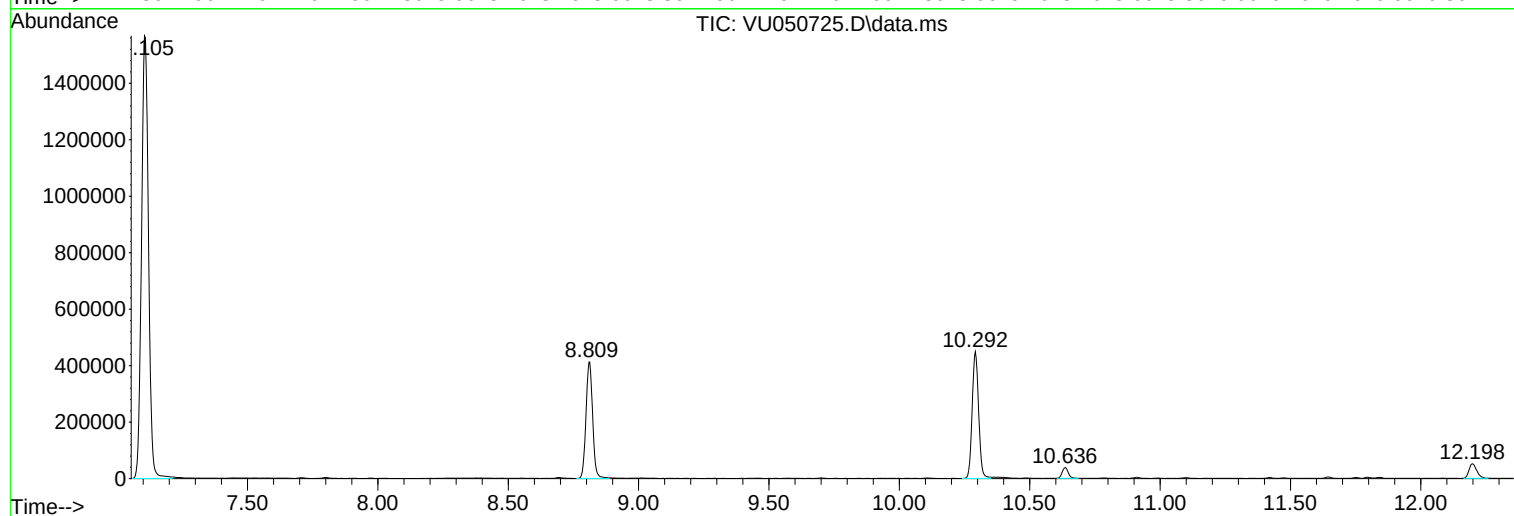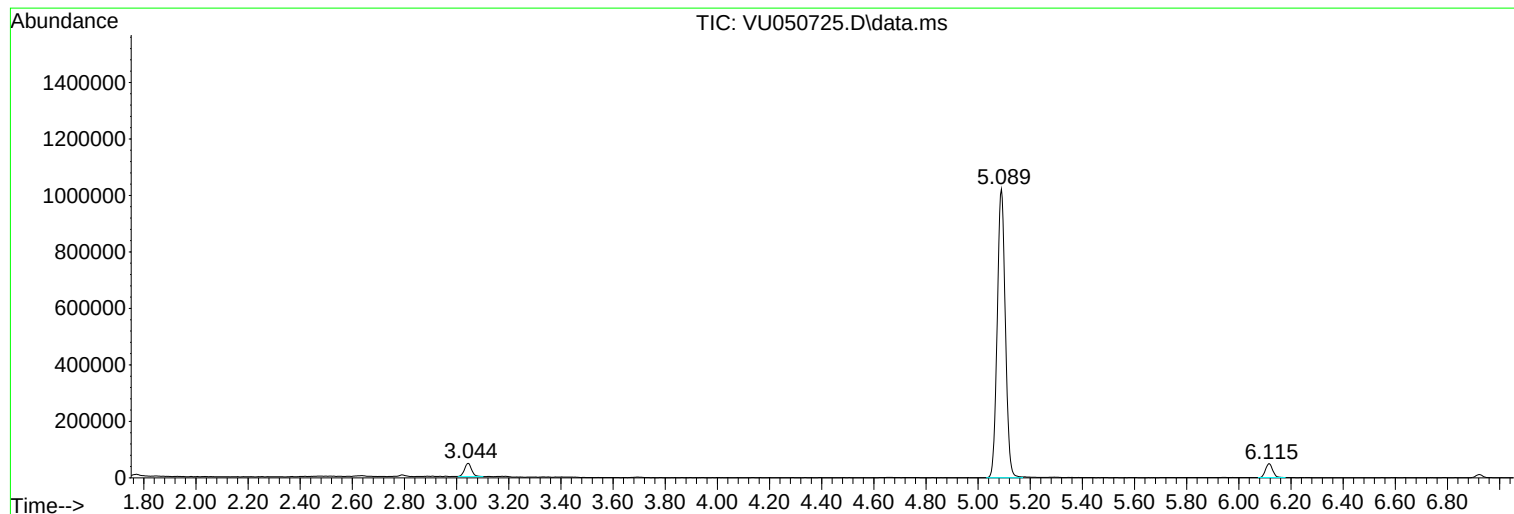

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
Data File : VU050725.D
Acq On : 16 Sep 2022 15:02
Operator : JC/MD
Sample : N4568-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38025-110121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091622\
Data File : VU050725.D
Acq On : 16 Sep 2022 15:02
Operator : JC/MD
Sample : N4568-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38025-110121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U081922DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------