

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091719\
 Data File : VU034613.D
 Acq On : 17 Sep 2019 14:15
 Operator : JC/SP
 Sample : K4838-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	88	94	104	rVB	81717	86657	10.75%	1.299%
2	1.672	175	181	190	rVB	66937	81192	10.07%	1.217%
3	2.257	356	363	377	rVB	150114	227822	28.26%	3.414%
4	3.128	632	634	635	rBV	520	268	0.03%	0.004%
5	3.244	666	670	673	rVB3	413	346	0.04%	0.005%
6	3.315	689	692	695	rBV3	644	452	0.06%	0.007%
7	3.350	700	703	705	rBV3	685	480	0.06%	0.007%
8	3.373	709	710	712	rVB	359	110	0.01%	0.002%
9	3.389	712	715	717	rBV	483	333	0.04%	0.005%
10	3.511	750	753	755	rBV2	390	258	0.03%	0.004%
11	3.546	761	764	766	rBV3	451	247	0.03%	0.004%
12	3.620	785	787	788	rBV2	375	131	0.02%	0.002%
13	3.633	789	791	798	rVB4	760	652	0.08%	0.010%
14	3.675	798	804	806	rBV4	561	606	0.08%	0.009%
15	3.694	808	810	813	rVB2	243	87	0.01%	0.001%
16	3.720	816	818	821	rBV3	452	308	0.04%	0.005%
17	3.842	852	856	860	rBV4	521	553	0.07%	0.008%
18	3.868	860	864	867	rBV3	456	431	0.05%	0.006%
19	3.910	876	877	882	rVB2	459	265	0.03%	0.004%
20	3.939	882	886	890	rBV4	580	553	0.07%	0.008%
21	3.961	890	893	896	rVB3	624	410	0.05%	0.006%
22	4.038	914	917	918	rBV2	385	197	0.02%	0.003%
23	4.064	922	925	927	rBV	369	219	0.03%	0.003%
24	4.151	941	952	985	rBV	90028	248534	30.83%	3.724%
25	4.624	1084	1099	1129	rBV2	130040	328407	40.73%	4.921%
26	4.939	1195	1197	1201	rBV3	612	408	0.05%	0.006%
27	5.096	1243	1246	1248	rBV3	387	279	0.03%	0.004%
28	5.135	1257	1258	1263	rBV	383	217	0.03%	0.003%
29	5.199	1276	1278	1279	rBV	291	136	0.02%	0.002%
30	5.222	1283	1285	1289	rVB2	1040	716	0.09%	0.011%
31	5.315	1289	1314	1346	rBV2	266998	806230	100.00%	12.081%
32	5.582	1394	1397	1399	rBV2	683	473	0.06%	0.007%
33	5.646	1415	1417	1420	rBV3	1183	710	0.09%	0.011%
34	5.710	1434	1437	1438	rBV	350	182	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091719\
 Data File : VU034613.D
 Acq On : 17 Sep 2019 14:15
 Operator : JC/SP
 Sample : K4838-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis

35	5.788	1458	1461	1462	rBV2	360	195	0.02%	0.003%
36	5.800	1462	1465	1466	rVV2	460	221	0.03%	0.003%
37	5.865	1471	1485	1508	rBV	282240	568693	70.54%	8.522%
38	6.193	1585	1587	1588	rBV2	348	129	0.02%	0.002%
39	6.308	1609	1623	1644	rBV3	197010	402178	49.88%	6.026%
40	6.540	1692	1695	1698	rBV3	765	630	0.08%	0.009%
41	6.659	1730	1732	1735	rBV3	400	245	0.03%	0.004%
42	6.697	1742	1744	1746	rVB2	459	154	0.02%	0.002%
43	6.810	1775	1779	1780	rBV3	529	299	0.04%	0.004%
44	6.849	1784	1791	1793	rBV5	1421	1814	0.22%	0.027%
45	6.913	1807	1811	1814	rBV3	745	572	0.07%	0.009%
46	6.961	1825	1826	1828	rVB	328	76	0.01%	0.001%
47	6.977	1829	1831	1834	rBV2	310	164	0.02%	0.002%
48	7.067	1853	1859	1861	rBV3	731	778	0.10%	0.012%
49	7.205	1888	1902	1930	rBV	111047	212667	26.38%	3.187%
50	7.543	1991	2007	2028	rBV	361152	650493	80.68%	9.747%
51	7.829	2086	2096	2124	rBV	76098	140752	17.46%	2.109%
52	8.099	2177	2180	2187	rBV3	753	640	0.08%	0.010%
53	8.228	2217	2220	2221	rBV2	476	309	0.04%	0.005%
54	8.289	2225	2239	2268	rBV	270655	528629	65.57%	7.921%
55	8.617	2336	2341	2345	rBV5	1131	1343	0.17%	0.020%
56	8.710	2366	2370	2372	rBV3	504	449	0.06%	0.007%
57	8.749	2376	2382	2384	rBV4	524	526	0.07%	0.008%
58	8.877	2419	2422	2426	rVB2	326	273	0.03%	0.004%
59	8.894	2426	2427	2428	rBV2	309	102	0.01%	0.002%
60	8.955	2444	2446	2447	rBV2	262	108	0.01%	0.002%
61	9.019	2462	2466	2468	rBV3	477	322	0.04%	0.005%
62	9.067	2468	2481	2514	rBV	414797	713634	88.51%	10.693%
63	9.273	2543	2545	2547	rBV2	609	376	0.05%	0.006%
64	9.447	2595	2599	2602	rBV2	454	383	0.05%	0.006%
65	9.492	2611	2613	2615	rBV2	233	138	0.02%	0.002%
66	9.585	2639	2642	2645	rBV2	287	160	0.02%	0.002%
67	9.656	2659	2664	2666	rBV3	353	331	0.04%	0.005%
68	9.820	2711	2715	2716	rBV	348	251	0.03%	0.004%
69	9.926	2745	2748	2749	rBV	527	297	0.04%	0.004%
70	9.993	2764	2769	2772	rBV	391	327	0.04%	0.005%
71	10.057	2785	2789	2791	rBV2	421	352	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091719\
 Data File : VU034613.D
 Acq On : 17 Sep 2019 14:15
 Operator : JC/SP
 Sample : K4838-16
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis

72	10.231	2841	2843	2845	rBV2	305	141	0.02%	0.002%
73	10.250	2847	2849	2851	rVV2	532	250	0.03%	0.004%
74	10.263	2851	2853	2857	rVV	373	184	0.02%	0.003%
75	10.318	2868	2870	2871	rBV	293	127	0.02%	0.002%
76	10.363	2881	2884	2886	rBV2	528	331	0.04%	0.005%
77	10.408	2886	2898	2917	rVV	279379	465132	57.69%	6.970%
78	10.588	2950	2954	2958	rBV3	587	533	0.07%	0.008%
79	10.717	2988	2994	2995	rBV3	692	581	0.07%	0.009%
80	10.755	3004	3006	3009	rBV3	530	261	0.03%	0.004%
81	10.794	3015	3018	3021	rBV	378	288	0.04%	0.004%
82	10.858	3036	3038	3041	rBV2	415	312	0.04%	0.005%
83	10.990	3077	3079	3081	rBV	221	101	0.01%	0.002%
84	11.012	3081	3086	3089	rBV2	567	498	0.06%	0.007%
85	11.070	3101	3104	3105	rVB3	312	177	0.02%	0.003%
86	11.196	3140	3143	3146	rVB3	317	220	0.03%	0.003%
87	11.212	3146	3148	3150	rBV2	285	134	0.02%	0.002%
88	11.398	3204	3206	3207	rBV2	407	155	0.02%	0.002%
89	11.459	3214	3225	3249	rBV	359012	606511	75.23%	9.088%
90	11.836	3331	3342	3361	rBV	345478	576662	71.53%	8.641%
91	12.414	3520	3522	3524	rBV	477	306	0.04%	0.005%
92	12.504	3548	3550	3556	rBV2	513	532	0.07%	0.008%
93	12.623	3583	3587	3591	rVB5	716	585	0.07%	0.009%
94	12.855	3654	3659	3662	rBV3	561	523	0.06%	0.008%
95	13.501	3855	3860	3862	rBV2	602	620	0.08%	0.009%
96	14.379	4131	4133	4136	rBV2	789	537	0.07%	0.008%


Sum of corrected areas: 6673580

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091719\
Data File : VU034613.D
Acq On : 17 Sep 2019 14:15
Operator : JC/SP
Sample : K4838-16
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

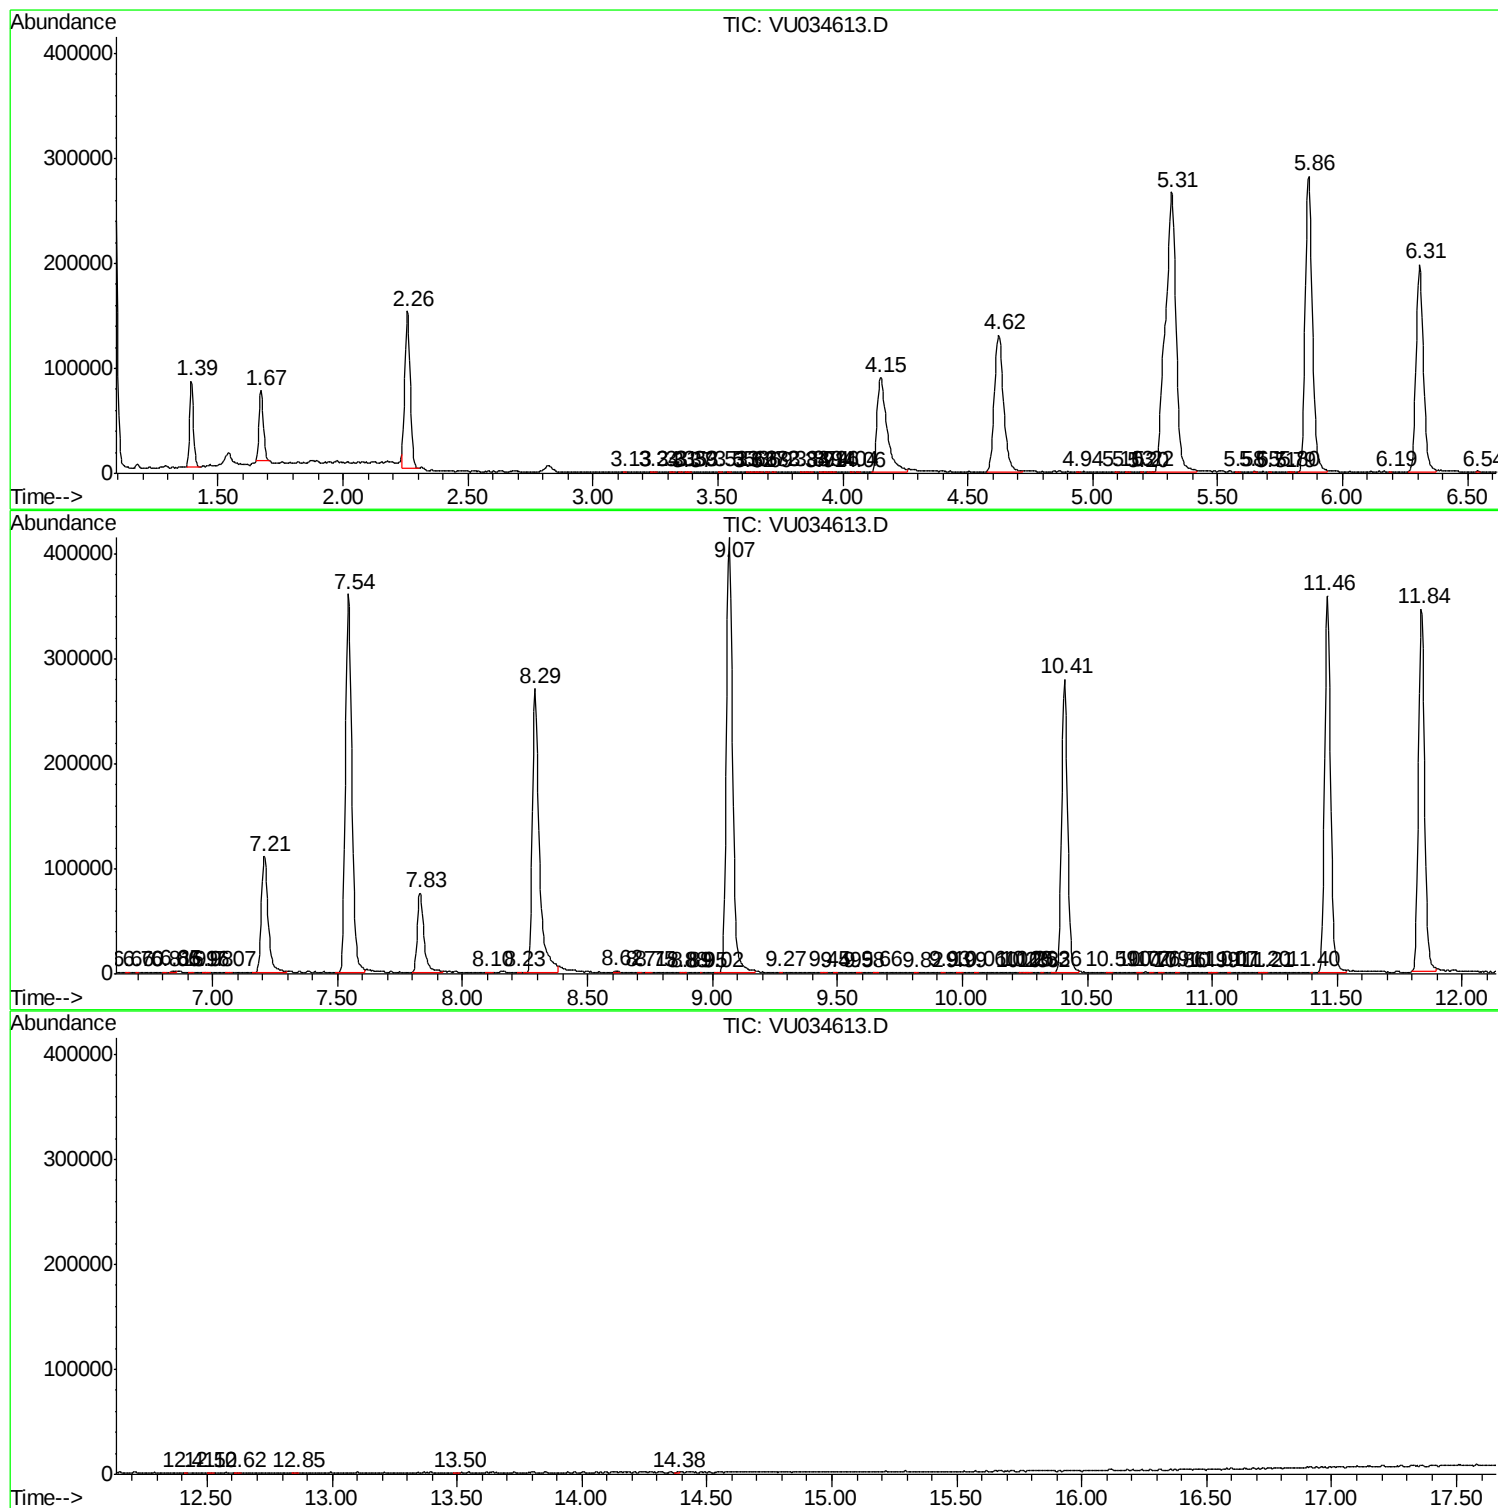

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091719\
Data File : VU034613.D
Acq On : 17 Sep 2019 14:15
Operator : JC/SP
Sample : K4838-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU091719\
Data File : VU034613.D
Acq On : 17 Sep 2019 14:15
Operator : JC/SP
Sample : K4838-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc