


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091719\
 Data File : VU034603.D
 Acq On : 17 Sep 2019 09:38
 Operator : JC/SP
 Sample : BFB33
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB33

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091619WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 18 13:00:12 2019

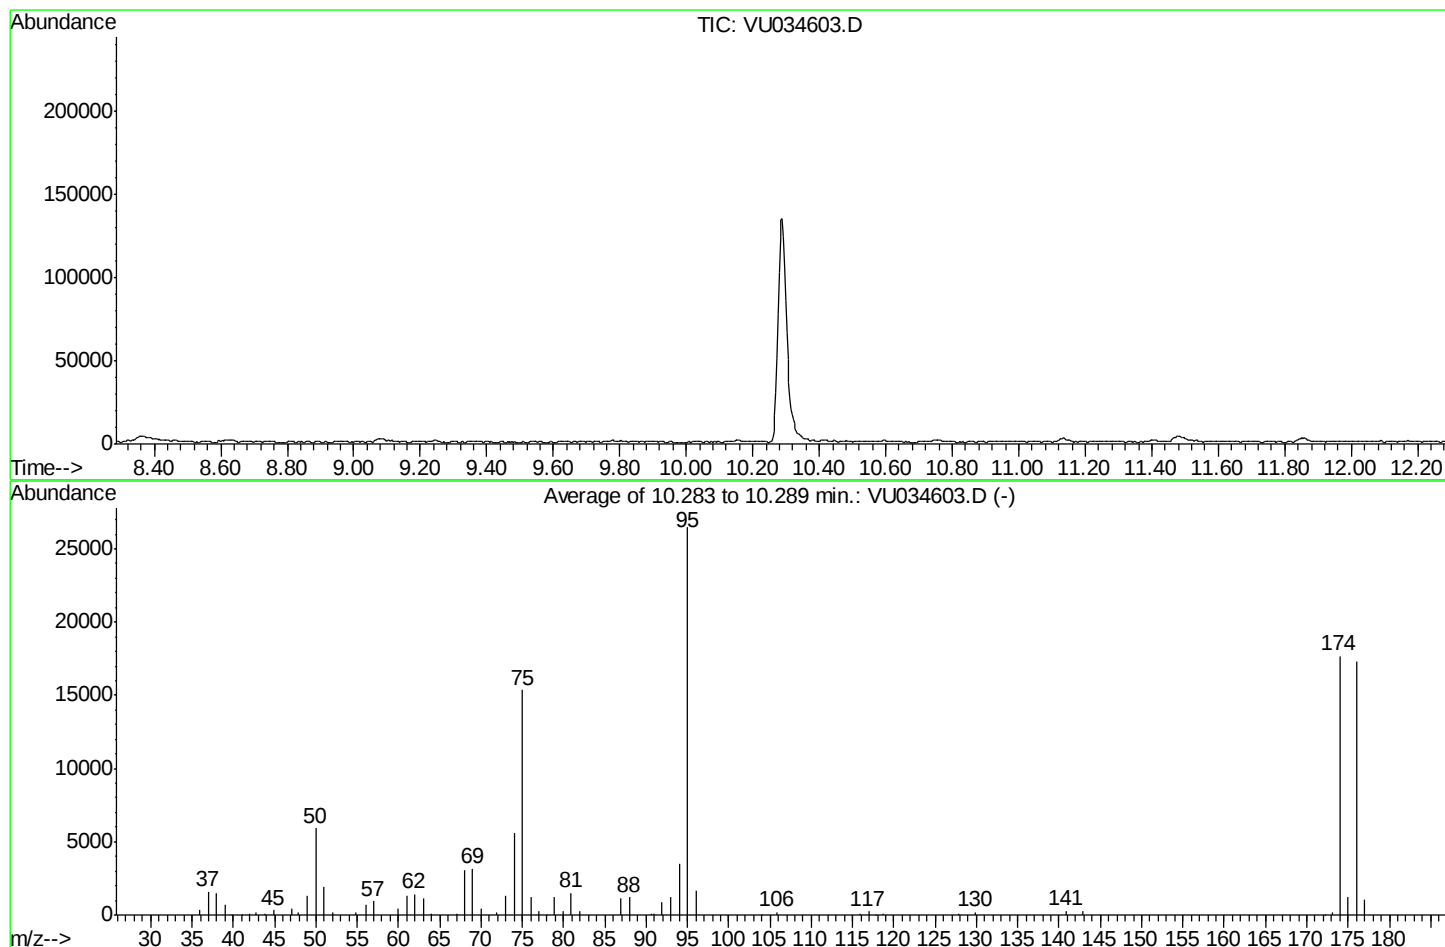

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	5942	PASS
75	95	30	80	58.0	15358	PASS
95	95	100	100	100.0	26469	PASS
96	95	5	9	6.4	1702	PASS
173	174	0.00	2	1.1	194	PASS
174	95	50	120	66.7	17666	PASS
175	174	5	9	7.0	1245	PASS
176	174	95	101	98.2	17343	PASS
177	176	5	9	6.3	1087	PASS

m/z	Abundance
36.00	375.0
37.00	1446.0
38.00	1381.0
39.00	710.0
39.90	176.0
41.10	102.0
41.90	147.0
42.80	238.0
43.90	914.0
44.90	280.0
47.00	415.0
48.00	204.0
49.00	1300.0
49.90	5699.0
51.00	1768.0
52.10	111.0
54.80	114.0
56.00	696.0
57.00	814.0
60.00	477.0
61.00	1243.0
62.00	1352.0
63.00	1111.0
64.00	109.0
68.00	2744.0
69.00	3026.0
70.00	367.0
71.90	124.0
73.00	1198.0
74.00	5538.0
75.00	14613.0
76.00	1182.0
77.10	189.0
78.80	1155.0
80.00	322.0
80.90	1348.0
82.00	334.0
86.90	988.0
88.00	1094.0
91.00	172.0
91.90	718.0
93.00	1158.0
94.00	3287.0
95.00	25456.0
96.00	1574.0
105.90	177.0
115.80	123.0
116.90	205.0
129.90	172.0
140.90	301.0
142.90	251.0
172.10	106.0
173.00	171.0
174.00	16632.0
175.00	1141.0
176.00	15679.0
176.90	975.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	311.0
37.00	1621.0
38.00	1506.0
39.00	784.0
39.90	161.0
41.10	120.0
42.00	124.0
42.80	216.0
43.90	821.0
44.90	317.0
47.10	458.0
47.90	201.0
49.00	1377.0
50.00	6151.0
51.00	1955.0
52.00	143.0
54.90	164.0
56.00	721.0
57.00	966.0
60.00	433.0
61.00	1308.0
61.90	1472.0
63.00	1191.0
64.00	143.0
67.00	111.0
68.00	3108.0
69.00	3288.0
70.00	427.0
72.00	201.0
73.00	1327.0
74.00	5763.0
75.00	15852.0
76.00	1235.0
77.00	263.0
78.90	1233.0
79.90	290.0
80.90	1528.0
81.90	308.0
86.90	1122.0
88.00	1269.0
90.70	141.0
91.90	922.0
92.90	1283.0
94.00	3585.0
95.00	27192.0
96.00	1715.0
105.90	227.0
115.80	134.0
116.90	255.0
118.70	141.0
127.80	127.0
129.90	218.0
140.90	260.0
143.00	235.0
173.00	206.0
174.00	18168.0
175.00	1247.0
176.00	17912.0
176.90	1132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.80	272.0
37.00	1725.0
37.90	1641.0
39.00	727.0
39.90	153.0
41.10	128.0
42.80	198.0
43.90	710.0
44.90	364.0
47.00	407.0
47.80	231.0
49.00	1359.0
50.00	5976.0
51.00	2013.0
52.00	164.0
54.90	203.0
56.00	642.0
57.00	1020.0
60.00	359.0
61.00	1304.0
61.90	1457.0
63.00	1163.0
64.00	141.0
67.00	119.0
67.90	3285.0
69.00	3260.0
70.00	408.0
72.00	235.0
73.00	1391.0
74.00	5437.0
75.00	15611.0
76.00	1371.0
77.00	306.0
77.90	123.0
78.90	1269.0
79.90	265.0
80.90	1624.0
81.90	284.0
87.00	1258.0
88.00	1267.0
90.70	159.0
91.90	1022.0
92.90	1319.0
94.00	3595.0
95.00	26760.0
96.00	1817.0
103.90	129.0
105.90	207.0
115.90	112.0
117.00	245.0
117.80	100.0
118.80	170.0
127.80	170.0
129.90	177.0
140.90	231.0
143.00	199.0
173.10	205.0
174.00	18200.0
175.00	1347.0
176.00	18440.0
176.90	1156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

Scan 2848 (10.247 min): VU034603.D
BFB33

m/z	Abundance
39.80	122.0
41.00	114.0
44.00	721.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33