


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU091720\
 Data File : VU040175.D
 Acq On : 17 Sep 2020 09:46
 Operator : SY/MD
 Sample : BFB03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Sep 18 04:01:22 2020

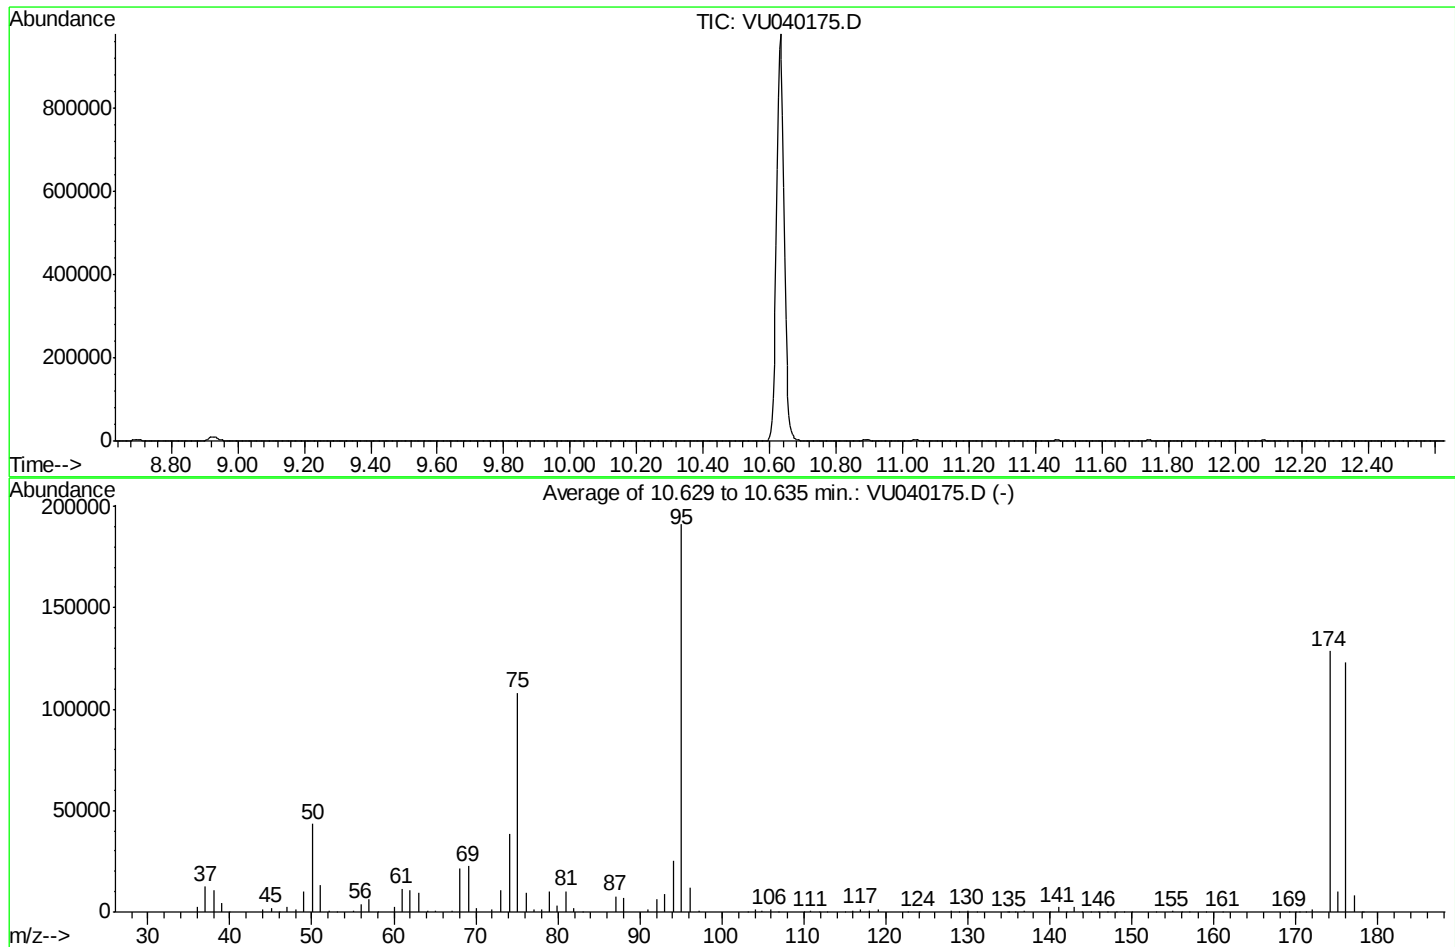

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	43274	PASS
75	95	30	80	56.5	108026	PASS
95	95	100	100	100.0	191104	PASS
96	95	5	9	6.4	12179	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.3	128538	PASS
175	174	5	9	7.8	9989	PASS
176	174	95	101	95.9	123325	PASS
177	176	5	9	6.7	8236	PASS

m/z	Abundance
36.00	2412.0
37.00	12812.0
38.00	11143.0
39.00	4572.0
40.00	190.0
44.00	1911.0
45.00	2272.0
46.10	283.0
47.00	2303.0
48.00	1538.0
49.10	10293.0
50.10	43984.0
51.00	13560.0
52.10	621.0
53.00	109.0
55.00	600.0
56.00	3950.0
57.00	6784.0
58.10	283.0
60.00	2638.0
61.00	11787.0
62.00	10900.0
63.00	9305.0
64.00	846.0
65.00	730.0
67.00	571.0
68.00	22168.0
69.10	21832.0
70.00	1663.0
72.00	1204.0
73.00	10877.0
74.10	38432.0
75.10	108544.0
76.10	9614.0
77.10	1060.0
78.00	989.0
78.90	10210.0
80.00	3162.0
81.00	10280.0
82.00	2309.0
82.90	297.0
87.00	7465.0
88.00	7096.0
91.00	957.0
92.10	6386.0
93.10	8956.0
94.10	24768.0
95.10	190784.0
96.10	12223.0
97.10	249.0
103.10	128.0
104.00	1199.0
104.90	354.0
105.90	1213.0
106.90	258.0
110.00	158.0
110.80	342.0
111.90	151.0
112.90	304.0
115.00	226.0
116.00	710.0
116.90	1677.0
118.00	883.0
119.00	1386.0
124.00	134.0
128.00	630.0
128.80	255.0
129.90	720.0
131.00	180.0
134.80	356.0
136.90	404.0
140.00	267.0
141.00	2582.0
142.10	277.0
143.00	2531.0
144.00	149.0
144.90	360.0
146.00	281.0
147.00	241.0
148.00	293.0
149.10	150.0
150.10	104.0
154.90	376.0
156.10	155.0
157.00	269.0
159.00	178.0
161.00	238.0
170.40	159.0
171.20	219.0
172.00	1081.0
174.10	125440.0
175.10	10163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

176.10

177.10

178.00

120136.0

8204.0

212.0

Instrument :

MSVOA_U

ClientSampleId :

BFB03

m/z	Abundance
36.10	2335.0
37.00	12873.0
38.00	11118.0
39.00	4732.0
40.10	229.0
44.10	1933.0
45.10	2137.0
46.10	333.0
47.00	2596.0
48.00	1473.0
49.10	10591.0
50.10	44808.0
51.00	13524.0
52.10	613.0
55.00	661.0
56.00	4035.0
57.00	6662.0
58.00	288.0
60.00	2494.0
61.00	12027.0
62.00	11244.0
63.10	9558.0
64.00	965.0
65.00	752.0
67.00	571.0
68.00	22200.0
69.10	23296.0
70.00	1710.0
72.00	1360.0
73.00	11015.0
74.10	39896.0
75.10	111704.0
76.10	9727.0
77.20	1028.0
78.00	1077.0
79.00	10732.0
79.90	3128.0
81.00	10515.0
81.90	2279.0
83.00	276.0
87.00	7776.0
88.00	7396.0
91.00	1040.0
92.10	6700.0
93.00	9468.0
94.10	25616.0
95.10	197312.0
96.10	12582.0
97.20	344.0
103.10	153.0
104.00	1211.0
104.90	344.0
105.90	1270.0
106.90	259.0
110.00	206.0
110.80	493.0
111.80	192.0
112.90	364.0
115.00	237.0
115.90	820.0
117.00	1519.0
118.00	951.0
119.00	1372.0
122.70	107.0
124.00	152.0
128.00	699.0
128.90	277.0
130.00	783.0
131.00	230.0
135.00	343.0
136.90	414.0
140.00	305.0
141.10	2665.0
142.10	271.0
143.00	2441.0
143.90	118.0
145.00	324.0
145.90	356.0
147.00	208.0
148.10	304.0
149.10	152.0
154.90	371.0
157.00	283.0
159.00	176.0
161.00	236.0
169.20	110.0
169.90	108.0
170.40	187.0
171.20	257.0
172.00	1101.0
174.10	133120.0
175.10	10392.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

176.10127648.0

177.108513.0

178.00182.0

Instrument :
MSVOA_U

ClientSampleId :
BFB03

m/z	Abundance
36.10	2047.0
37.00	11542.0
38.00	9899.0
39.00	4396.0
40.10	265.0
44.10	1705.0
45.10	1770.0
46.00	327.0
47.00	2572.0
48.00	1387.0
49.00	9499.0
50.10	41032.0
51.00	12264.0
52.00	532.0
55.00	625.0
56.00	3688.0
57.00	5998.0
58.00	257.0
60.00	2224.0
61.00	10845.0
62.00	10765.0
63.10	8696.0
64.10	951.0
65.00	647.0
67.10	531.0
68.00	20080.0
69.00	22768.0
70.10	1716.0
72.00	1335.0
73.00	9964.0
74.10	37072.0
75.10	103832.0
76.10	8864.0
77.20	856.0
78.00	926.0
79.00	10260.0
79.90	2854.0
81.00	9877.0
81.90	2096.0
83.00	244.0
87.00	7510.0
88.00	6843.0
91.00	984.0
92.10	6264.0
93.00	9095.0
94.10	24536.0
95.10	185216.0
96.10	11734.0
97.10	419.0
103.10	127.0
104.00	1102.0
104.90	333.0
105.90	1115.0
106.80	195.0
110.00	239.0
110.80	444.0
111.80	204.0
112.80	310.0
115.00	236.0
115.90	820.0
117.00	1376.0
118.00	900.0
119.00	1252.0
124.00	132.0
128.00	698.0
129.00	316.0
130.00	781.0
131.00	293.0
135.00	325.0
135.80	100.0
136.90	421.0
140.00	243.0
141.10	2313.0
142.00	249.0
143.00	2217.0
145.10	288.0
145.90	360.0
146.90	174.0
148.10	349.0
149.10	119.0
149.90	119.0
153.00	109.0
154.90	322.0
157.10	276.0
159.10	135.0
161.10	193.0
170.40	192.0
171.20	228.0
172.00	1029.0
174.10	127056.0
175.10	9414.0
176.10	122192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

177.107992.0

178.20192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

Scan 2875 (10.584 min): VU040175.D
BFB03

m/z	Abundance
40.00	123.0
43.90	355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03