

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
 Data File : VU044684.D
 Acq On : 17 Sep 2021 14:17
 Operator : SY/MD
 Sample : M3739-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG6

Quant Time: Sep 18 01:33:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 18 01:28:45 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

SAM
 9/18/2021 11:23:57 AM

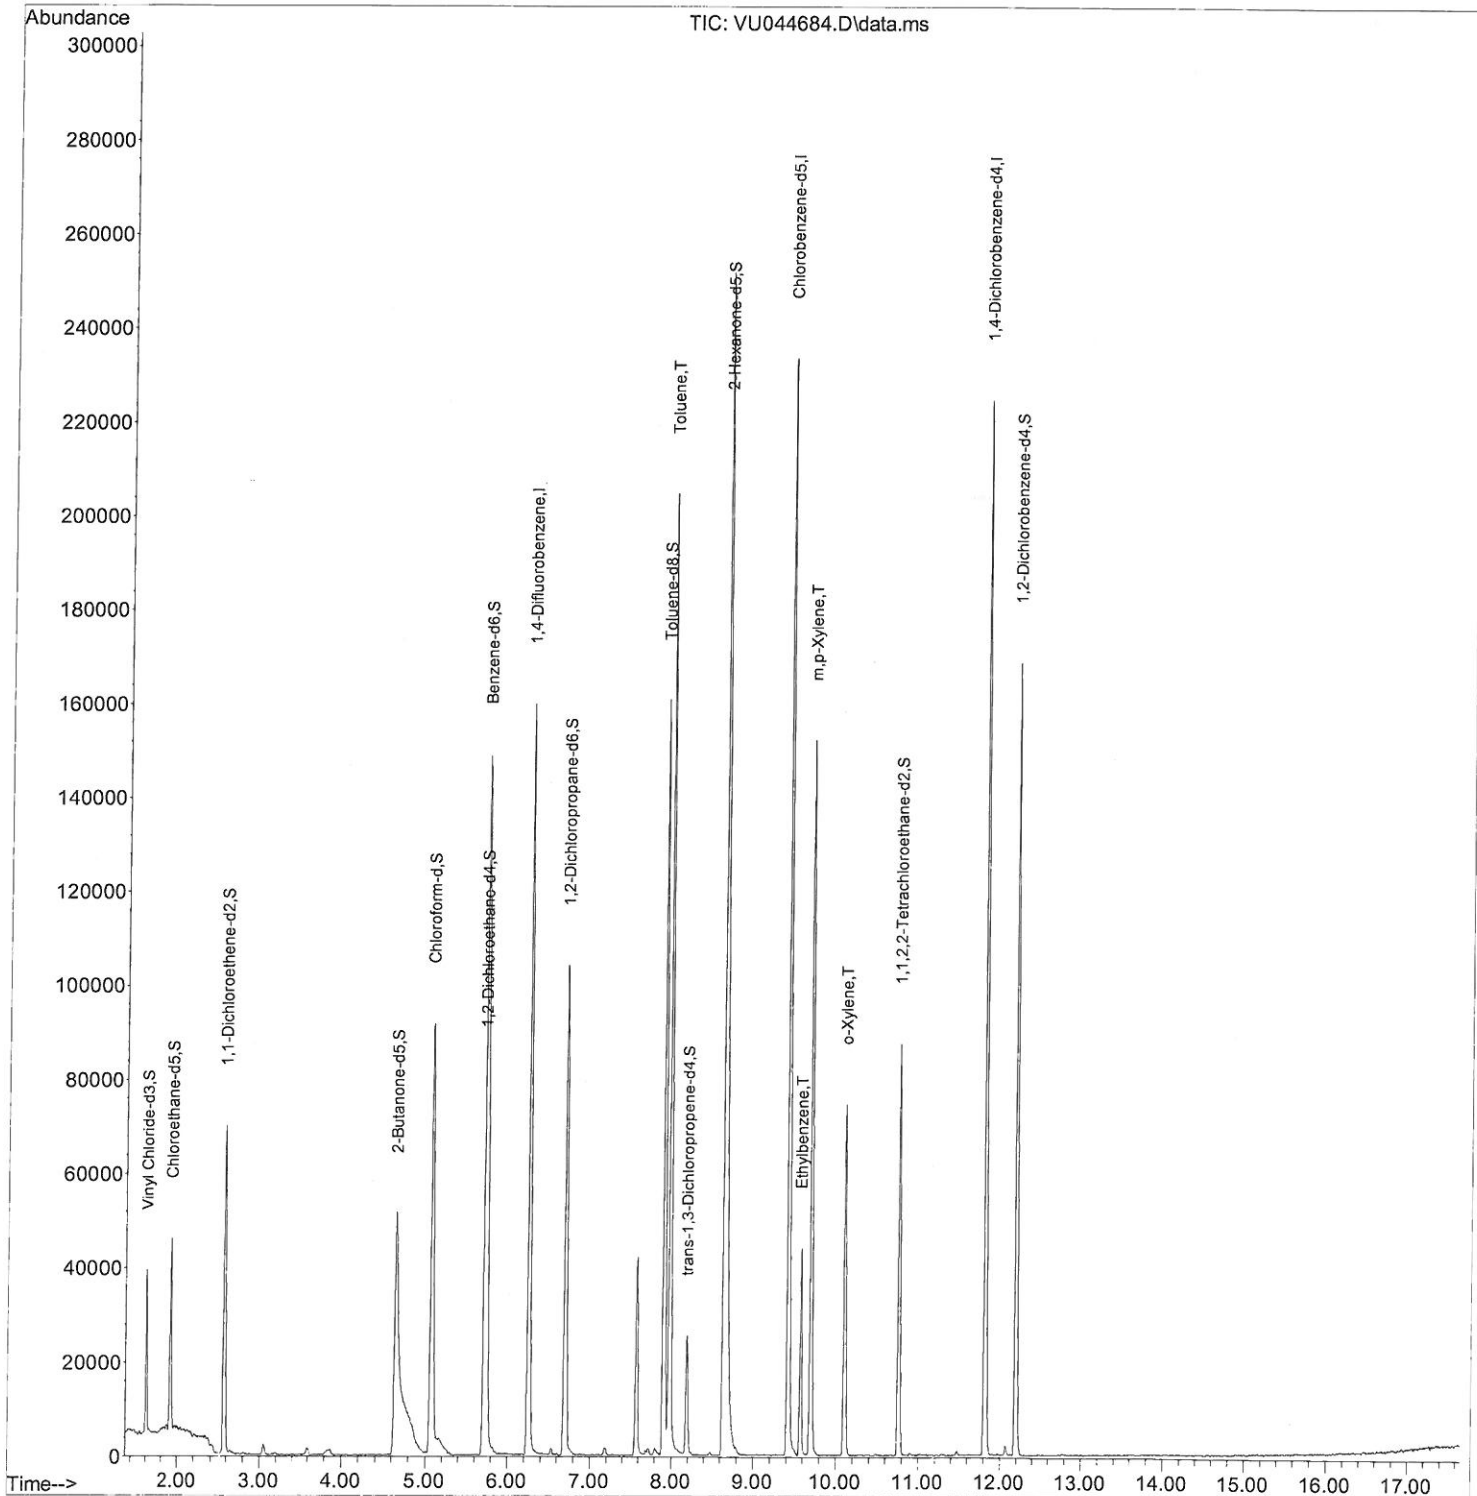

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
 Data File : VU044684.D
 Acq On : 17 Sep 2021 14:17
 Operator : SY/MD
 Sample : M3739-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG6

Quant Time: Sep 18 01:33:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 18 01:28:45 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

SAM
 9/18/2021 11:23:57 AM

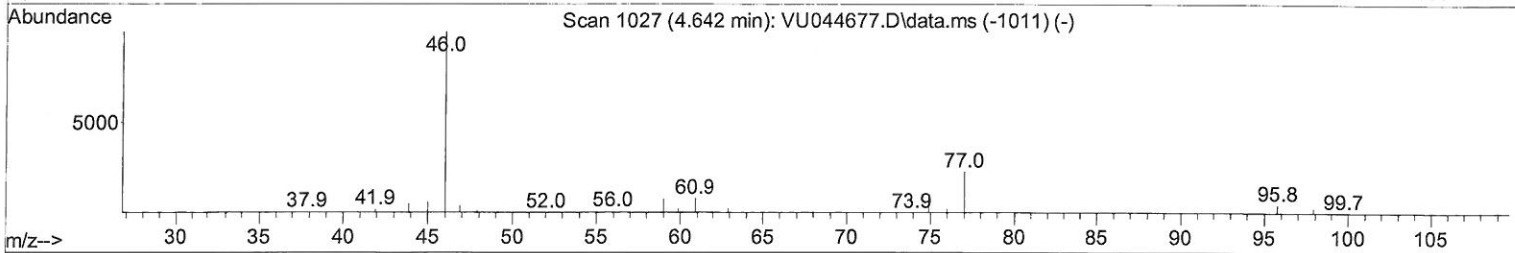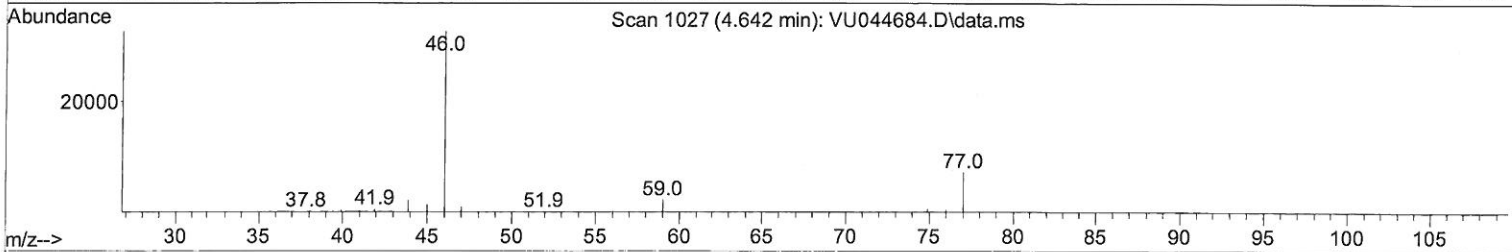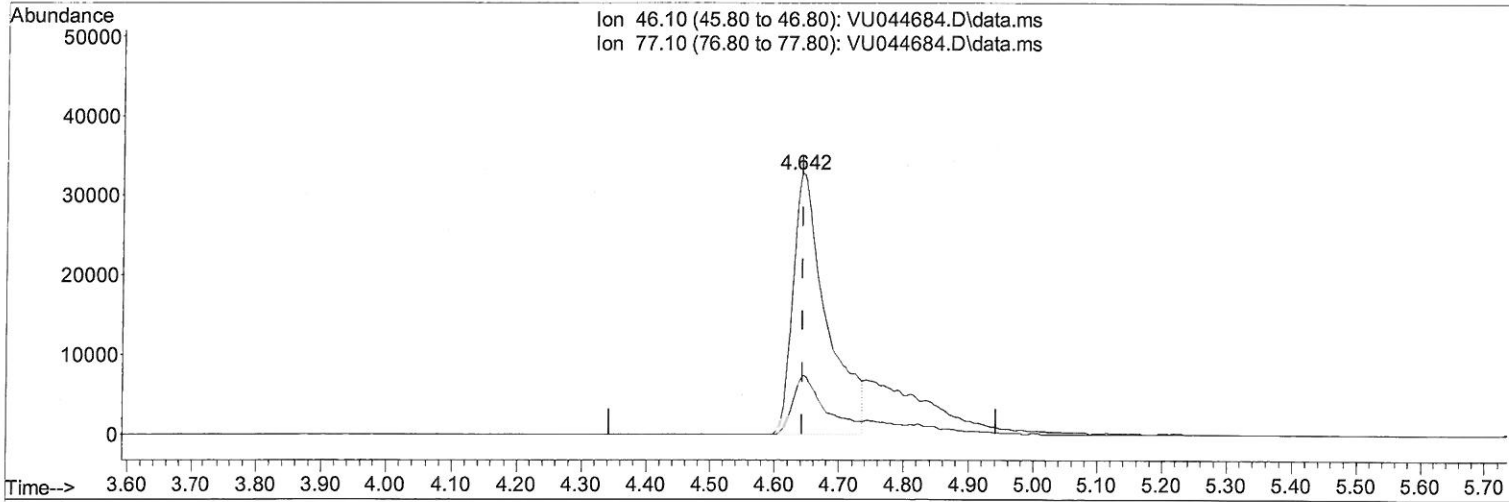

TIC: VU044684.D\data.ms

(20) 2-Butanone-d5 (S)

4.642min (+ 0.000) 39.13 ug/L

response 118649

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.40	21.94
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044684.D
Acq On : 17 Sep 2021 14:17
Operator : SY/MD
Sample : M3739-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG6

Quant Time: Sep 18 01:33:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 18 01:28:45 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

SAM
9/18/2021 11:23:57 AM

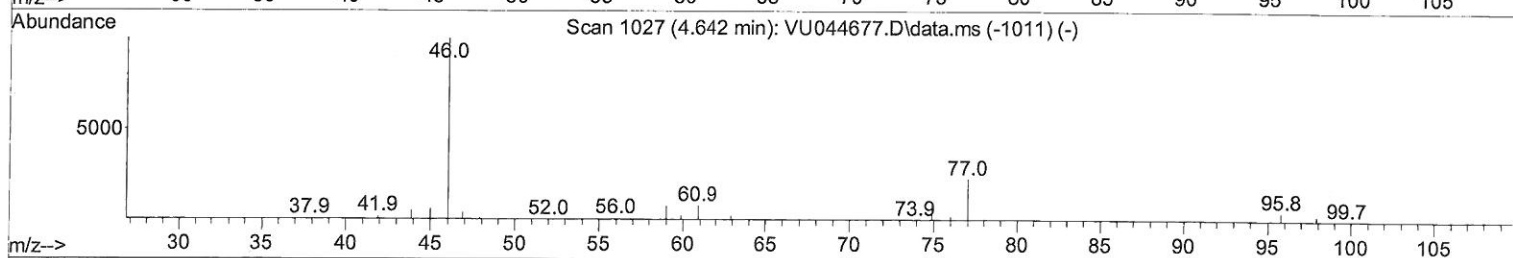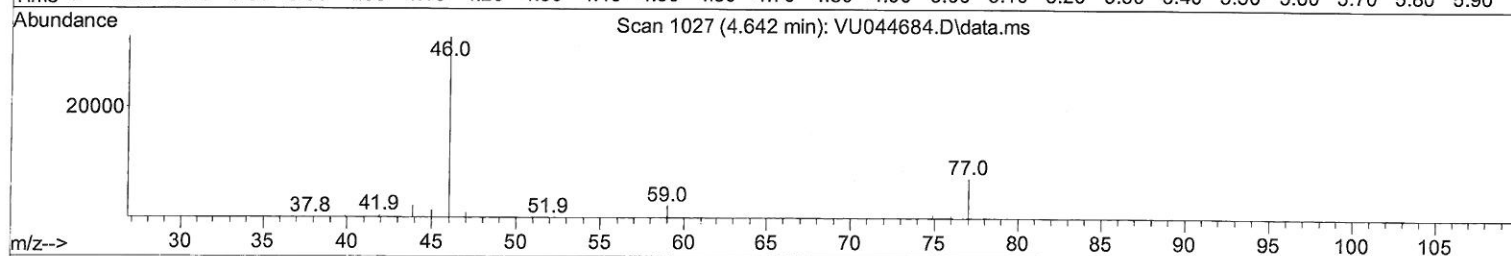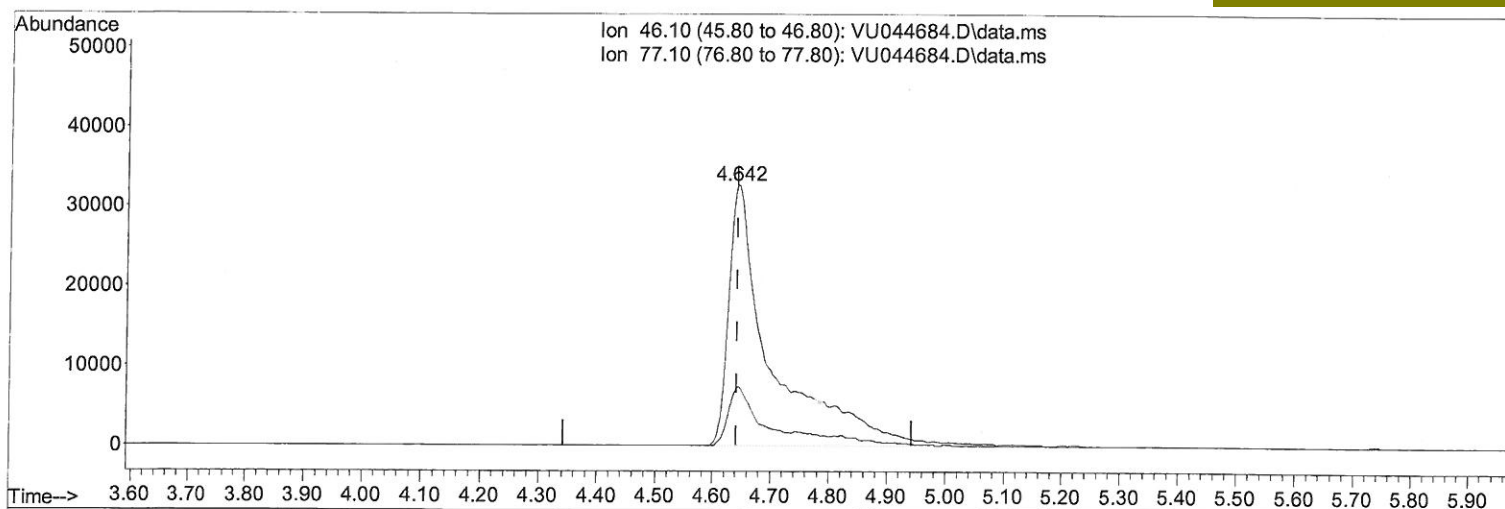

TIC: VU044684.D\data.ms

(20) 2-Butanone-d5 (S)

4.642min (+ 0.000) 54.86 ug/L m

response 166344

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	17.40	15.65
0.00	0.00	0.00
0.00	0.00	0.00

MD
09/21/21

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
 Data File : VU044684.D
 Acq On : 17 Sep 2021 14:17
 Operator : SY/MD
 Sample : M3739-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0AG6

Quant Time: Sep 18 01:33:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 18 01:28:45 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

SAM
 9/18/2021 11:23:57 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	122596	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	122813	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	54241	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	24174	3.342	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 66.800%			
7) Chloroethane-d5	1.919	69	29067	3.937	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 78.800%			
11) 1,1-Dichloroethene-d2	2.572	65	13853	3.792	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 75.800%			
20) 2-Butanone-d5	4.642	46	166344m	54.857	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 109.720%			
24) Chloroform-d	5.073	84	71488	4.698	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 94.000%			
26) 1,2-Dichloroethane-d4	5.710	65	42747	4.712	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 94.200%			
32) Benzene-d6	5.735	84	131793	4.209	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 84.200%			
36) 1,2-Dichloropropane-d6	6.697	67	47983	4.666	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 93.400%			
41) Toluene-d8	7.903	98	102615	3.764	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 75.200%			
43) trans-1,3-Dichloroprop...	8.185	79	14149	3.903	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 78.000%			
46) 2-Hexanone-d5	8.645	63	119769	51.405	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 102.800%			
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44430	4.872	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 97.400%			
66) 1,2-Dichlorobenzene-d4	12.198	152	39332	4.395	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 87.800%			
Target Compounds						
					Qvalue	
42) Toluene	7.976	91	146677	3.853	ug/L	100
52) Ethylbenzene	9.574	91	30024	0.728	ug/L	98
53) m,p-Xylene	9.697	106	41718	2.661	ug/L	99
54) o-Xylene	10.105	106	19283	1.287	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed