

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
 Data File : VU044682.D
 Acq On : 17 Sep 2021 13:28
 Operator : SY/MD
 Sample : M3739-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG0

Quant Time: Sep 18 01:33:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 18 01:28:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	121552	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	123763	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	53591	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	23825	3.322	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.400%
7) Chloroethane-d5	1.919	69	28875	3.945	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.000%
11) 1,1-Dichloroethene-d2	2.572	65	12519	3.456	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.200%
20) 2-Butanone-d5	4.642	46	157964	52.541	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.080%
24) Chloroform-d	5.070	84	69874	4.632	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.600%
26) 1,2-Dichloroethane-d4	5.710	65	42387	4.712	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.200%
32) Benzene-d6	5.736	84	129308	4.098	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	6.700	67	46829	4.519	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.400%
41) Toluene-d8	7.903	98	98749	3.595	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.800%
43) trans-1,3-Dichloroprop...	8.186	79	13607	3.725	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.400%
46) 2-Hexanone-d5	8.645	63	115280	49.099	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.200%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	42326	4.606	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	12.198	152	38422	4.345	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.800%
Target Compounds					Qvalue	
13) Acetone	2.649	43	8634	4.409	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044682.D
Acq On : 17 Sep 2021 13:28
Operator : SY/MD
Sample : M3739-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG0

Quant Time: Sep 18 01:33:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 18 01:28:45 2021
Response via : Initial Calibration

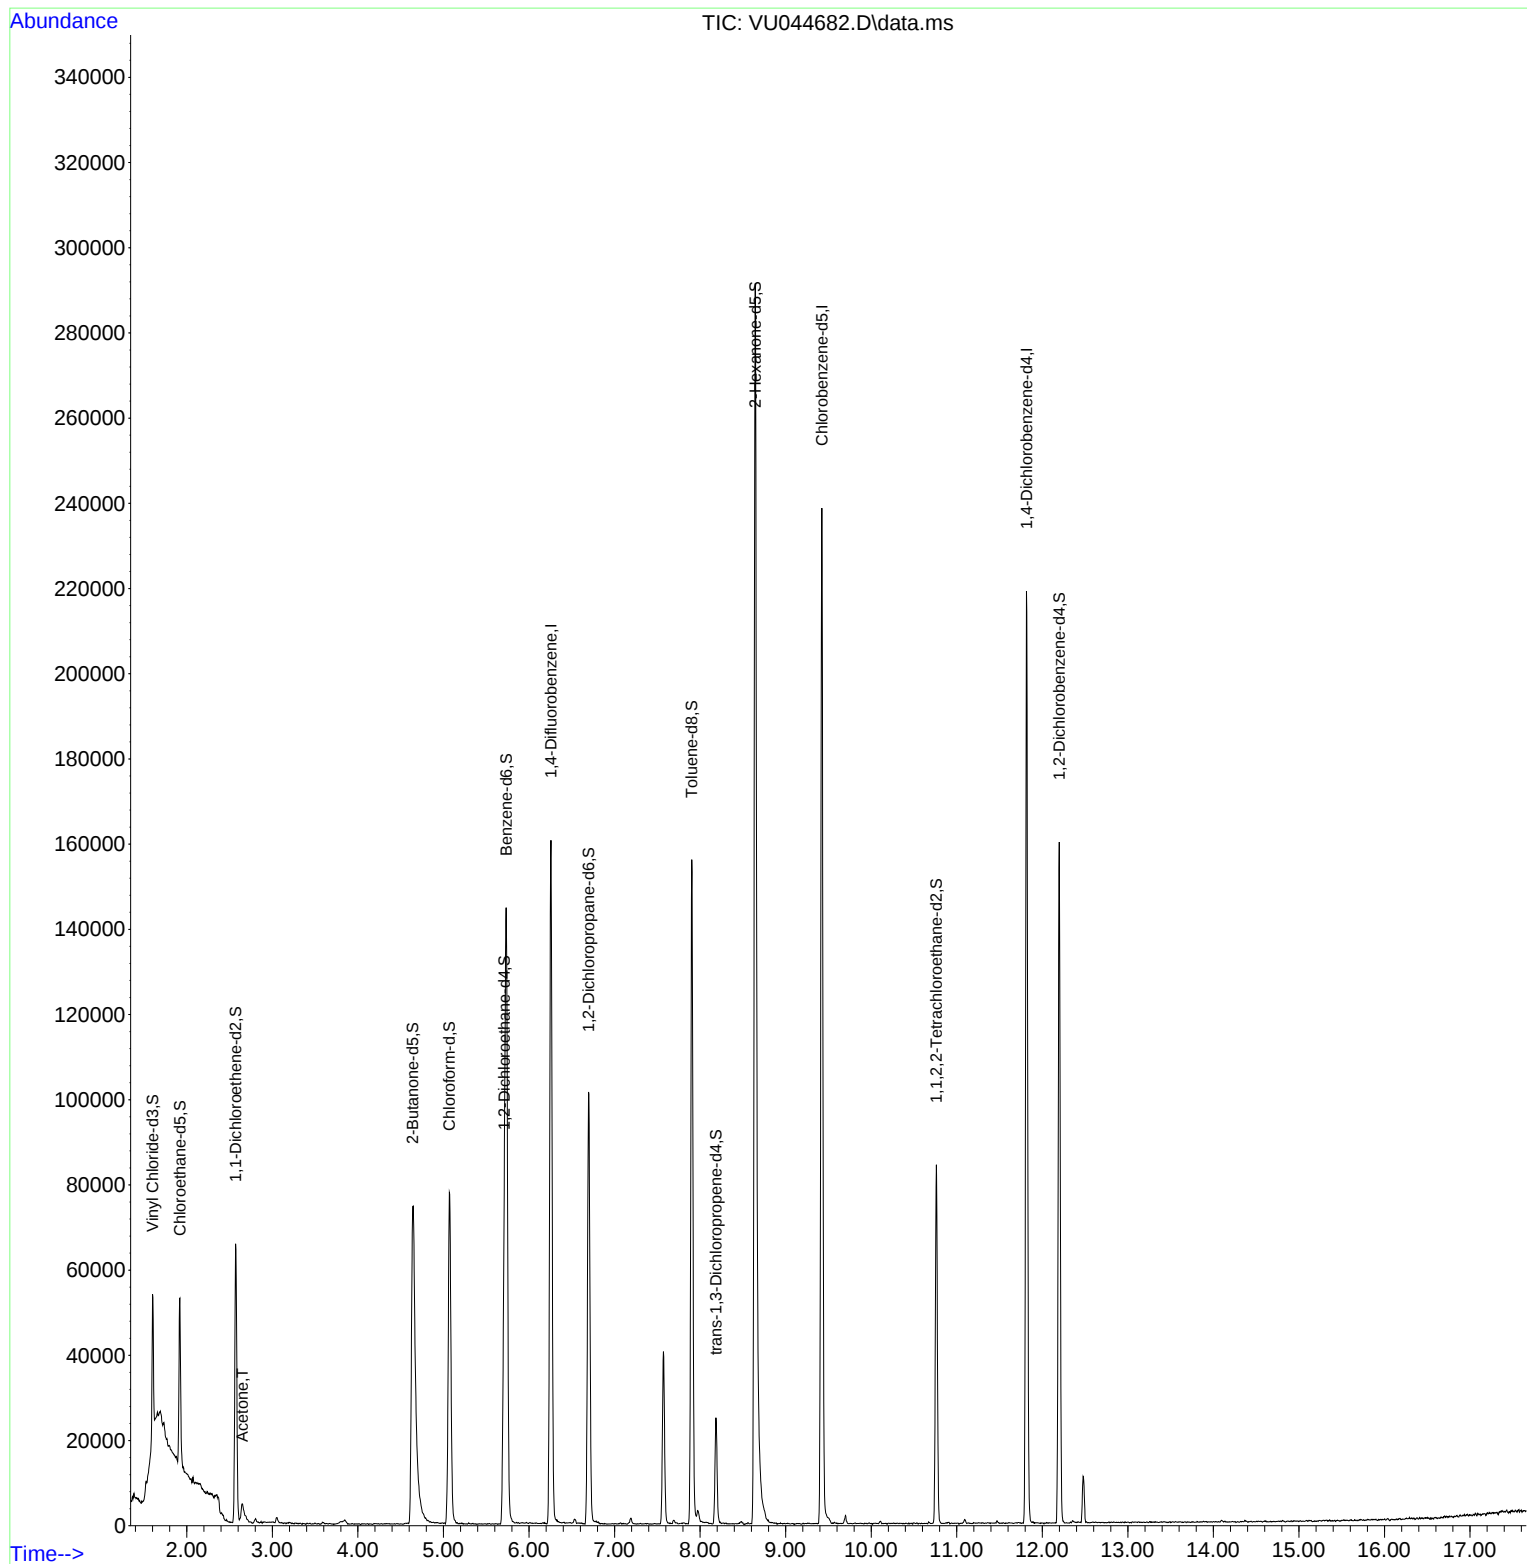

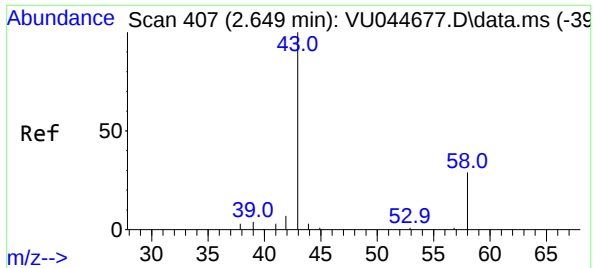

#13
Acetone
Concen: 4.409 ug/L
RT: 2.649 min Scan# 407
Delta R.T. 0.000 min
Lab File: VU044682.D
Acq: 17 Sep 2021 13:28

Instrument :
MSVOA_U
ClientSampleId :
C0AG0

Tgt Ion: 43 Resp: 8634
Ion Ratio Lower Upper
43 100
58 30.3 0.0 42.4

