

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
 Data File : VU044683.D
 Acq On : 17 Sep 2021 13:53
 Operator : SY/MD
 Sample : M3739-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG1

Quant Time: Sep 18 01:33:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 18 01:28:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	120572	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	122330	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	52160	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	24383	3.427	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.600%
7) Chloroethane-d5	1.919	69	29559	4.071	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	2.575	65	13054	3.633	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	4.642	46	166151	55.714	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.420%
24) Chloroform-d	5.073	84	72026	4.813	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
26) 1,2-Dichloroethane-d4	5.710	65	43930	4.923	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	5.735	84	129752	4.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.200%
36) 1,2-Dichloropropane-d6	6.697	67	48662	4.750	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.000%
41) Toluene-d8	7.906	98	101458	3.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.800%
43) trans-1,3-Dichloroprop...	8.185	79	13822	3.828	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.600%
46) 2-Hexanone-d5	8.645	63	117361	50.570	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.140%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	44370	4.885	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.800%
66) 1,2-Dichlorobenzene-d4	12.198	152	39215	4.556	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%
Target Compounds						Qvalue
13) Acetone	2.649	43	8362	4.305	ug/L	99
33) Benzene	5.780	78	4756	0.131	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044683.D
Acq On : 17 Sep 2021 13:53
Operator : SY/MD
Sample : M3739-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG1

Quant Time: Sep 18 01:33:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 18 01:28:45 2021
Response via : Initial Calibration




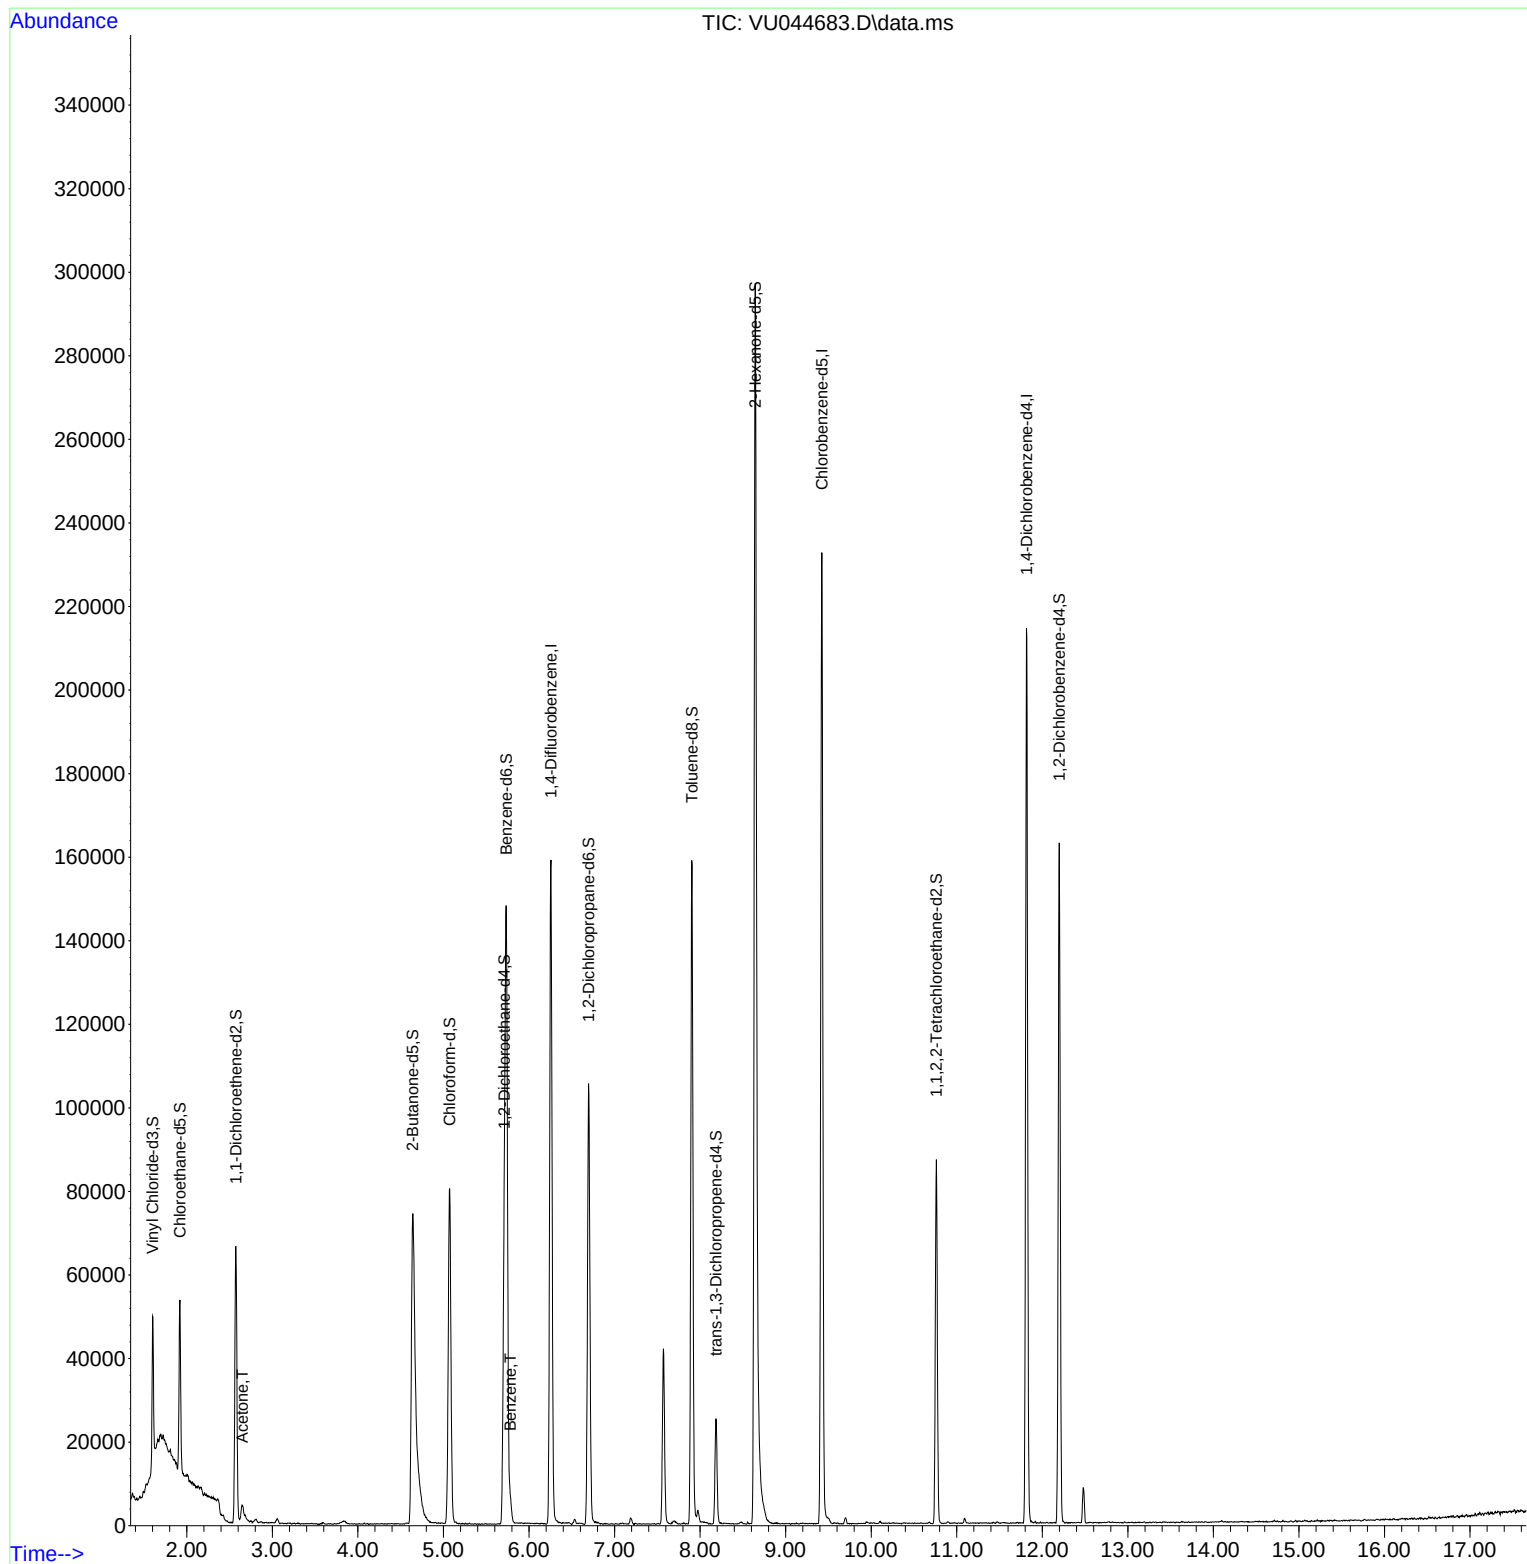


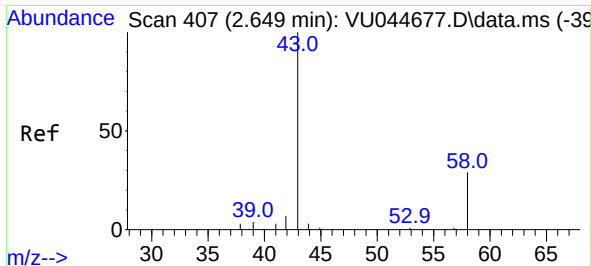

#13
Acetone
Concen: 4.305 ug/L
RT: 2.649 min Scan# 407
Delta R.T. 0.000 min
Lab File: VU044683.D
Acq: 17 Sep 2021 13:53

Instrument :
MSVOA_U
ClientSampled :
C0AG1

Tgt Ion: 43 Resp: 8362
Ion Ratio Lower Upper
43 100
58 20.7 0.0 42.4

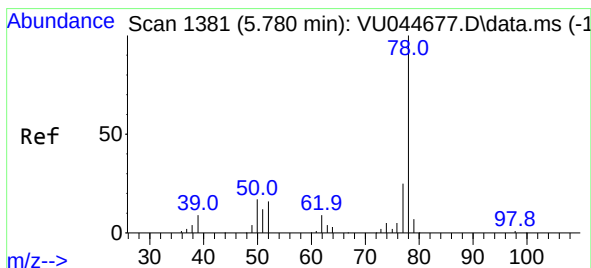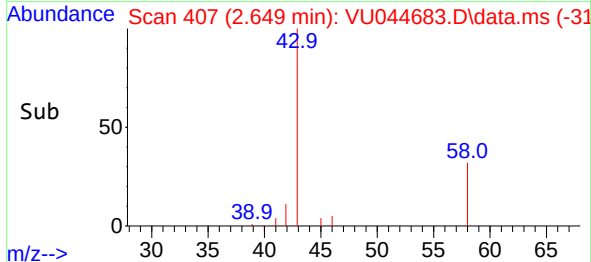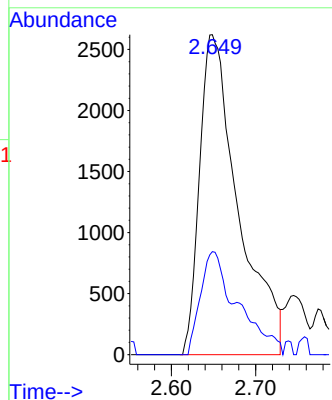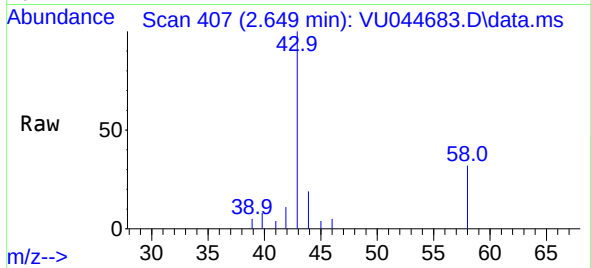

#33
Benzene
Concen: 0.131 ug/L
RT: 5.780 min Scan# 1381
Delta R.T. 0.000 min
Lab File: VU044683.D
Acq: 17 Sep 2021 13:53

Tgt Ion: 78 Resp: 4756

