

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
 Data File : VU044685.D
 Acq On : 17 Sep 2021 14:41
 Operator : SY/MD
 Sample : M3777-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B62

Quant Time: Sep 18 01:34:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 18 01:28:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	120818	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.424	117	121939	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	52322	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	23164	3.249	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.000%
7) Chloroethane-d5	1.919	69	28288	3.888	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.800%
11) 1,1-Dichloroethene-d2	2.572	65	13170	3.658	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	4.646	46	163388	54.676	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.360%
24) Chloroform-d	5.070	84	69711	4.649	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	5.710	65	42690	4.775	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%
32) Benzene-d6	5.736	84	127219	4.092	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
36) 1,2-Dichloropropane-d6	6.697	67	47420	4.644	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.800%
41) Toluene-d8	7.903	98	97882	3.616	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.400%
43) trans-1,3-Dichloroprop...	8.186	79	13743	3.818	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%
46) 2-Hexanone-d5	8.645	63	115014	49.718	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.440%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	42134	4.654	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.000%
66) 1,2-Dichlorobenzene-d4	12.198	152	37611	4.356	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.200%
Target Compounds						Qvalue
13) Acetone	2.646	43	2562	1.316	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044685.D
Acq On : 17 Sep 2021 14:41
Operator : SY/MD
Sample : M3777-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B62


Quant Time: Sep 18 01:34:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 18 01:28:45 2021
Response via : Initial Calibration

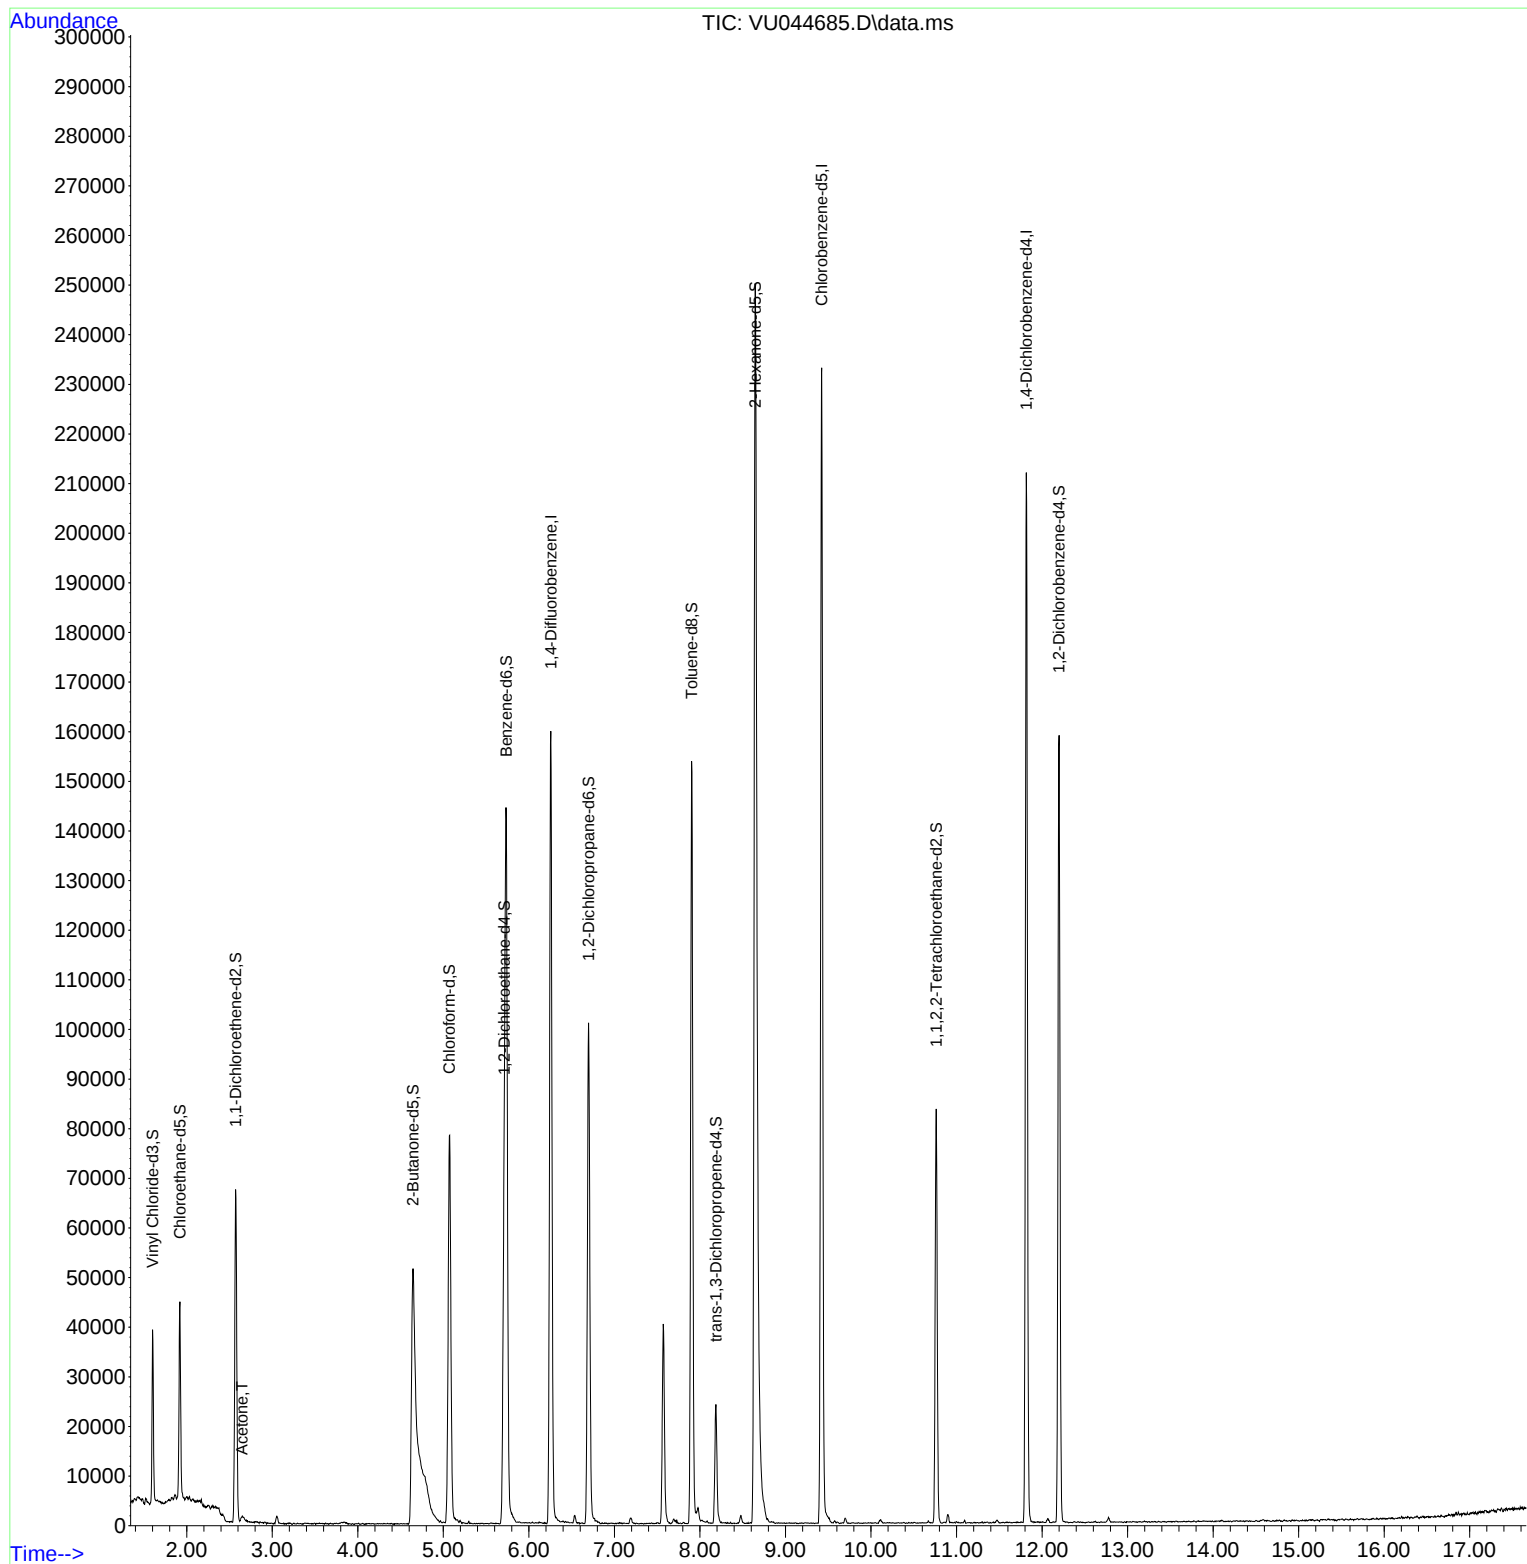

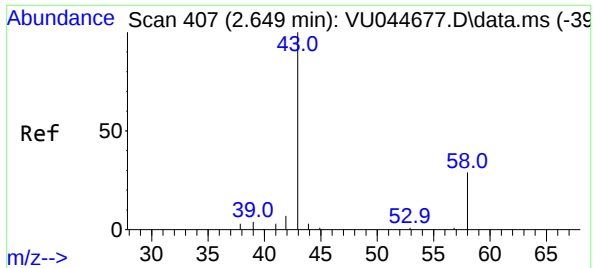

#13
 Acetone
 Concen: 1.316 ug/L
 RT: 2.646 min Scan# 406
 Delta R.T. -0.003 min
 Lab File: VU044685.D
 Acq: 17 Sep 2021 14:41

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B62

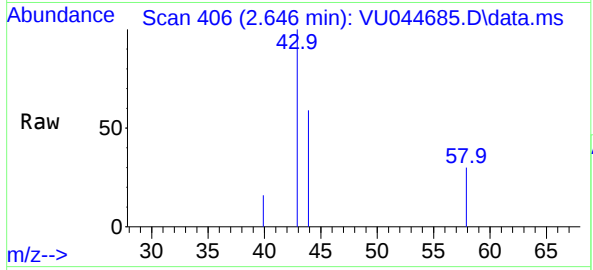

Tgt Ion: 43	Resp: 2562
Ion Ratio	Lower Upper
43	100
58	20.8 0.0 42.4

