

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
 Data File : VU044679.D
 Acq On : 17 Sep 2021 12:16
 Operator : SY/MD
 Sample : M3763-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	95	rVB	34608	40087	6.60%	1.098%
2	1.919	171	180	193	rBV	39913	53360	8.78%	1.462%
3	2.572	371	383	398	rBV	68012	111669	18.37%	3.059%
4	2.655	398	409	429	rVV2	3176	8866	1.46%	0.243%
5	4.649	1013	1029	1048	rBV	47586	159958	26.32%	4.381%
6	5.073	1144	1161	1180	rBV	77894	174201	28.66%	4.772%
7	5.732	1345	1366	1392	rBV2	144220	387852	63.81%	10.624%
8	6.256	1515	1529	1552	rBV	161256	303876	50.00%	8.324%
9	6.697	1653	1666	1685	rBV	99855	197771	32.54%	5.417%
10	7.571	1927	1938	1957	rBV	39545	71813	11.82%	1.967%
11	7.903	2028	2041	2056	rBV	153392	267897	44.08%	7.338%
12	7.977	2056	2064	2078	rVB	15104	25579	4.21%	0.701%
13	8.186	2118	2129	2152	rBV2	24021	42730	7.03%	1.170%
14	8.649	2258	2273	2312	rBV	238379	607776	100.00%	16.648%
15	8.796	2312	2319	2334	rVB6	4399	8677	1.43%	0.238%
16	9.423	2501	2514	2544	rBV	236124	399860	65.79%	10.953%
17	9.697	2590	2599	2611	rBV2	6104	9460	1.56%	0.259%
18	10.118	2714	2730	2742	rBV3	15956	27996	4.61%	0.767%
19	10.761	2919	2930	2948	rVB	84511	137583	22.64%	3.769%
20	11.816	3246	3258	3275	rBV	220198	355911	58.56%	9.749%
21	12.198	3364	3377	3397	rVB	159060	257865	42.43%	7.063%


Sum of corrected areas: 3650787

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044679.D
Acq On : 17 Sep 2021 12:16
Operator : SY/MD
Sample : M3763-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

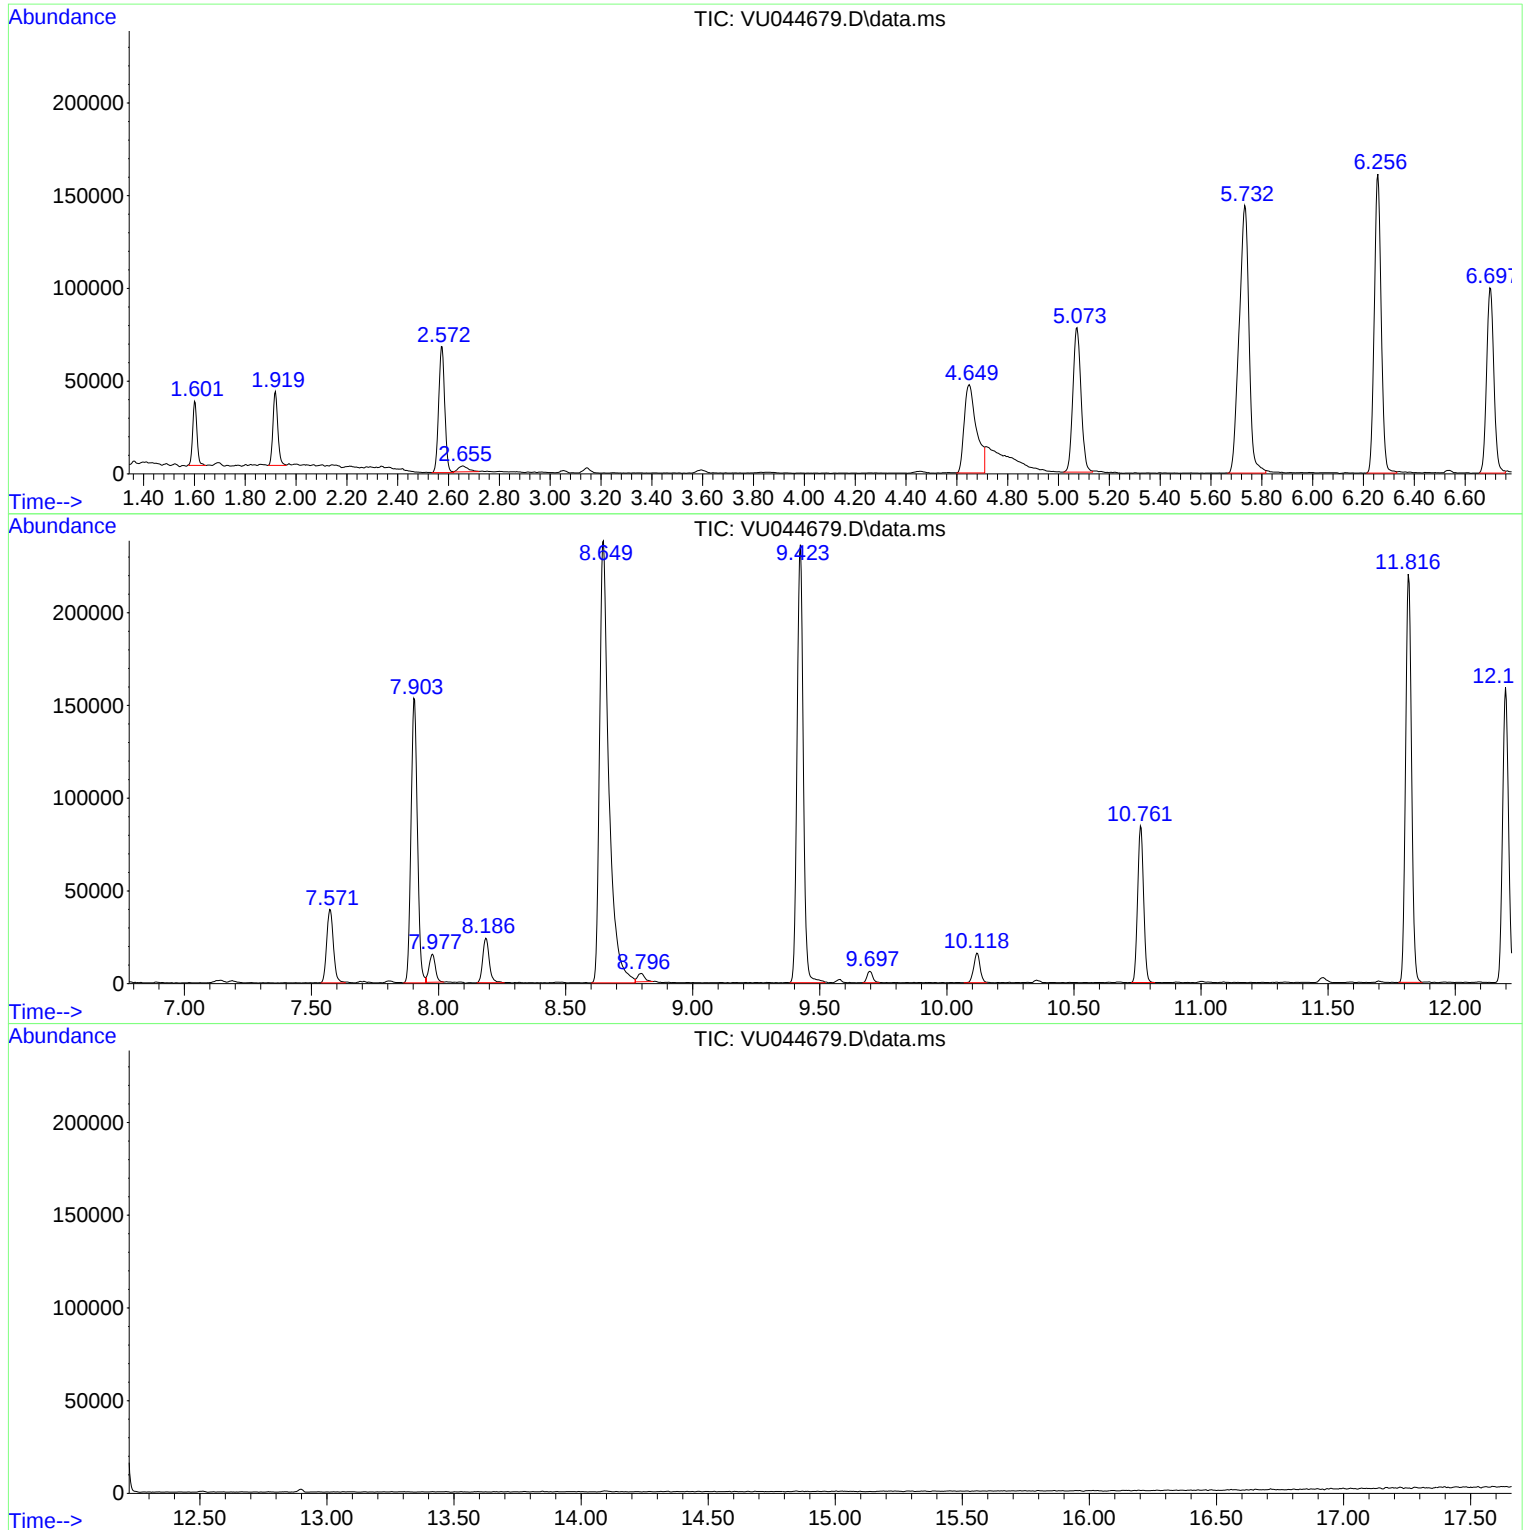

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044679.D
Acq On : 17 Sep 2021 12:16
Operator : SY/MD
Sample : M3763-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044679.D
Acq On : 17 Sep 2021 12:16
Operator : SY/MD
Sample : M3763-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
