


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091721\
Data File : VU044676.D
Acq On : 17 Sep 2021 10:14
Operator : SY/MD
Sample : BFB020
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB020

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090921WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 18 01:28:45 2021

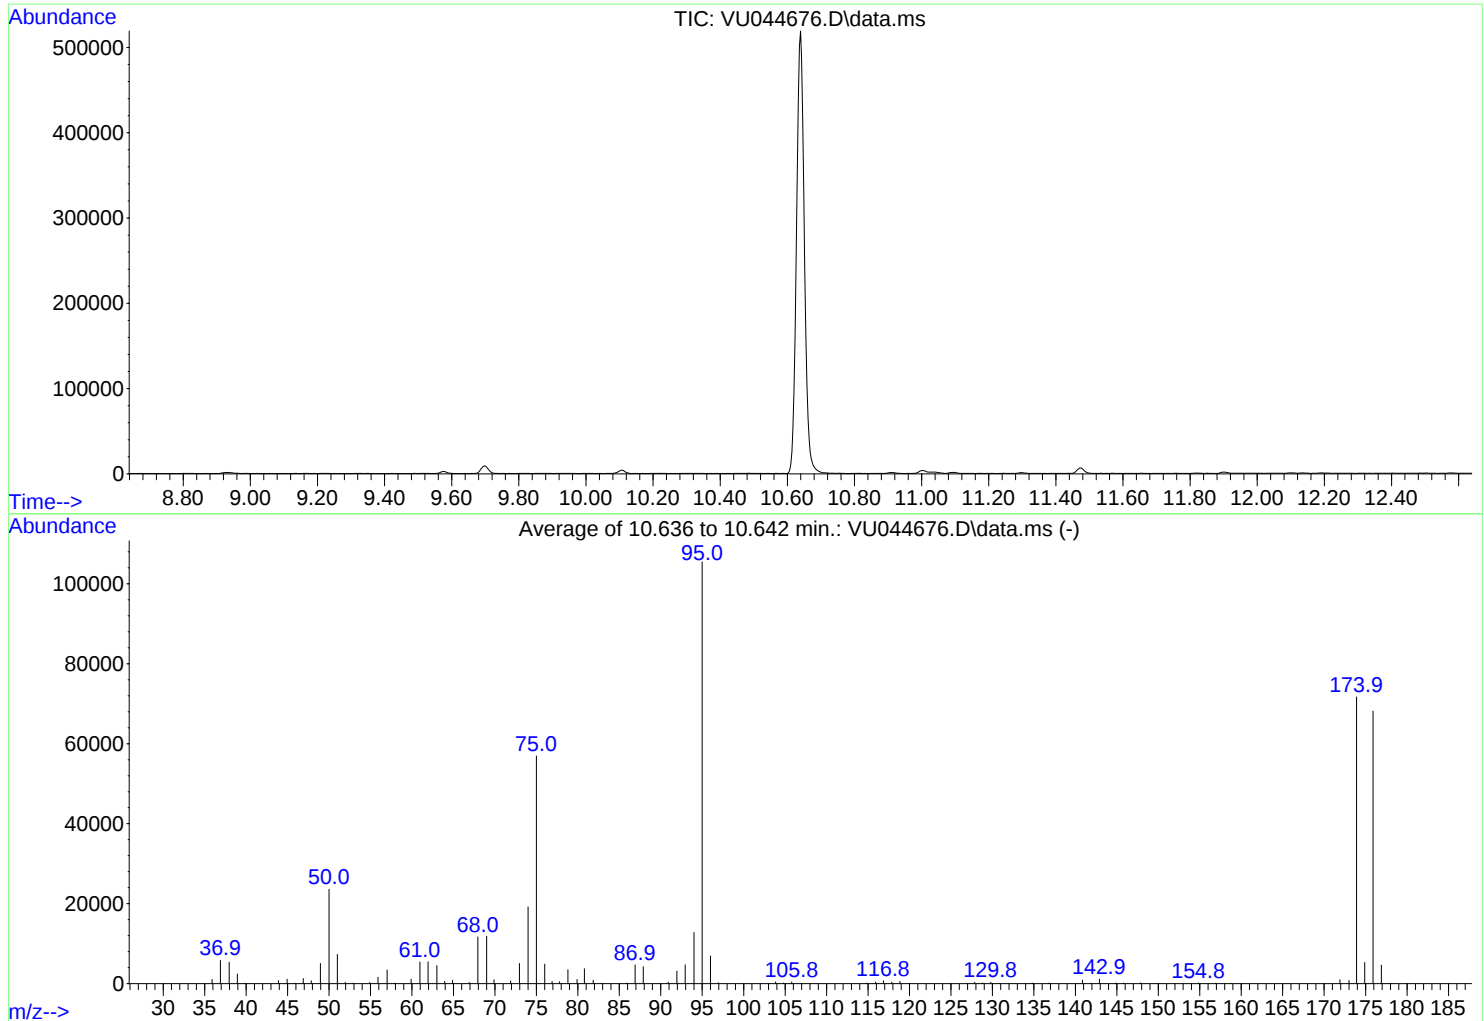

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.4	23613	PASS
75	95	30	80	54.0	56941	PASS
95	95	100	100	100.0	105491	PASS
96	95	5	9	6.5	6906	PASS
173	174	0.00	2	1.1	817	PASS
174	95	50	120	68.0	71701	PASS
175	174	5	9	7.4	5298	PASS
176	174	95	101	95.1	68195	PASS
177	176	5	9	6.8	4657	PASS

m/z	Abundance
35.90	1045.0
36.90	5652.0
37.90	5084.0
38.90	2388.0
39.80	209.0
43.90	1122.0
44.90	1127.0
45.80	133.0
46.90	1199.0
47.90	689.0
48.90	4838.0
50.00	22784.0
51.00	6808.0
51.90	341.0
52.90	129.0
54.90	333.0
55.90	1479.0
57.00	3196.0
57.90	124.0
59.90	1205.0
60.90	5107.0
61.90	5233.0
63.00	4389.0
63.90	552.0
64.90	802.0
66.90	295.0
68.00	11424.0
69.00	11152.0
69.90	877.0
71.90	704.0
73.00	4871.0
74.00	18496.0
75.00	54536.0
76.00	4639.0
76.90	519.0
77.80	516.0
78.80	3329.0
79.90	1018.0
80.80	3582.0
81.90	843.0
82.90	136.0
85.80	152.0
86.90	4549.0
87.90	4177.0
90.90	391.0
92.00	2947.0
93.00	4745.0
94.00	12132.0
95.00	101752.0
96.00	6769.0
96.90	240.0
103.80	439.0
104.80	119.0
105.80	402.0
114.80	130.0
115.90	386.0
116.80	687.0
117.90	377.0
118.80	532.0
127.80	355.0
128.80	157.0
129.80	387.0
130.80	119.0
134.80	147.0
136.80	160.0
140.80	830.0
142.00	103.0
142.90	1183.0
144.80	132.0
145.80	149.0
147.90	222.0
154.80	203.0
156.90	148.0
171.90	905.0
173.10	814.0
173.90	71880.0
174.90	5192.0
175.90	67560.0
176.90	4416.0
177.80	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	1082.0
36.90	6001.0
38.00	5537.0
38.90	2492.0
39.80	202.0
43.90	1149.0
44.90	1188.0
45.80	128.0
46.90	1356.0
47.90	751.0
48.90	5238.0
50.00	24280.0
51.00	7583.0
51.90	341.0
52.90	137.0
54.90	350.0
55.90	1633.0
57.00	3550.0
57.90	146.0
59.90	1167.0
60.90	5597.0
61.90	5631.0
63.00	4728.0
64.00	598.0
64.90	864.0
66.90	318.0
68.00	12022.0
69.00	12196.0
69.90	1005.0
71.90	730.0
72.90	5173.0
74.00	19824.0
75.00	58800.0
76.00	4996.0
76.90	574.0
77.80	518.0
78.80	3604.0
79.90	1044.0
80.80	3888.0
81.80	851.0
82.90	122.0
85.90	156.0
86.90	4844.0
87.90	4398.0
90.90	407.0
92.00	3275.0
93.00	4817.0
94.00	13232.0
95.00	108784.0
96.00	7116.0
96.90	232.0
103.90	442.0
104.80	163.0
105.80	475.0
107.00	114.0
114.80	139.0
115.90	414.0
116.80	720.0
117.90	418.0
118.90	611.0
127.90	375.0
128.80	150.0
129.80	384.0
130.80	110.0
134.80	167.0
136.80	166.0
140.80	885.0
141.90	110.0
142.90	1219.0
144.90	155.0
145.80	170.0
147.80	220.0
154.90	198.0
156.90	152.0
158.80	109.0
171.90	972.0
173.00	821.0
173.90	73976.0
174.90	5483.0
175.90	70392.0
176.90	4847.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
39.80	112.0
43.90	382.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
35.90	1060.0
36.90	5792.0
38.00	5513.0
39.00	2315.0
39.80	190.0
43.90	1127.0
45.00	1099.0
45.80	111.0
46.90	1293.0
47.80	755.0
49.00	5068.0
50.00	23776.0
51.00	7594.0
52.00	318.0
52.90	112.0
54.90	328.0
55.90	1694.0
57.00	3519.0
57.90	146.0
59.90	1022.0
61.00	5528.0
62.00	5526.0
63.00	4501.0
64.00	566.0
64.90	876.0
66.90	296.0
67.90	11558.0
69.00	12143.0
69.90	1002.0
71.90	657.0
72.90	5100.0
74.00	19336.0
75.00	57488.0
76.00	5007.0
76.90	642.0
77.80	429.0
78.80	3488.0
79.90	1010.0
80.80	3730.0
81.80	803.0
86.00	171.0
86.90	4714.0
87.90	4170.0
90.90	406.0
91.90	3205.0
92.90	4586.0
94.00	13053.0
95.00	105936.0
96.00	6833.0
97.00	186.0
103.80	439.0
104.80	167.0
105.80	473.0
106.90	105.0
114.80	123.0
115.90	382.0
116.90	718.0
117.80	401.0
118.90	594.0
127.90	336.0
128.80	157.0
129.80	333.0
134.80	178.0
136.80	161.0
140.90	944.0
141.80	110.0
142.90	1148.0
144.90	191.0
145.80	165.0
147.80	199.0
149.80	102.0
154.90	182.0
156.90	124.0
158.80	107.0
171.90	996.0
172.90	817.0
173.90	69248.0
174.90	5219.0
175.90	66632.0
176.90	4708.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020