




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091724\
Data File : VU060834.D
Acq On : 17 Sep 2024 15:42
Operator : MD/SY
Sample : P3973-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/18/2024
Supervised By :Semsettin Yesilyurt 09/18/2024

Quant Time: Sep 18 01:18:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 18 01:15:55 2024
Response via : Initial Calibration

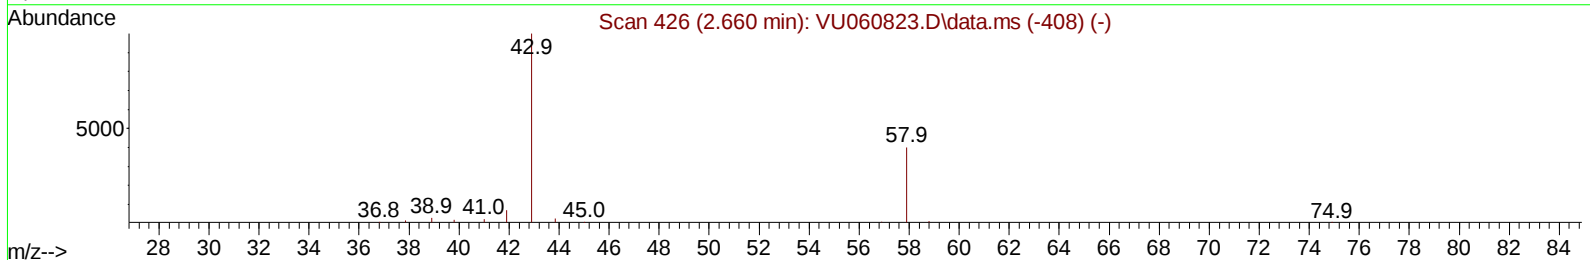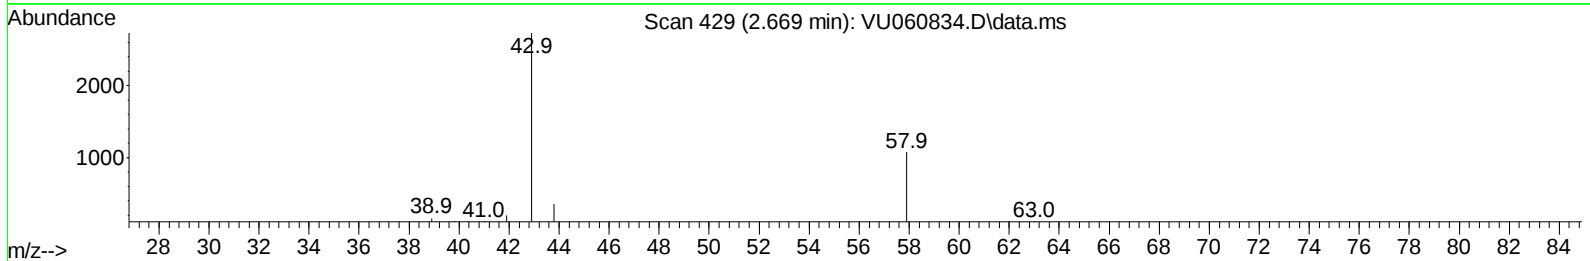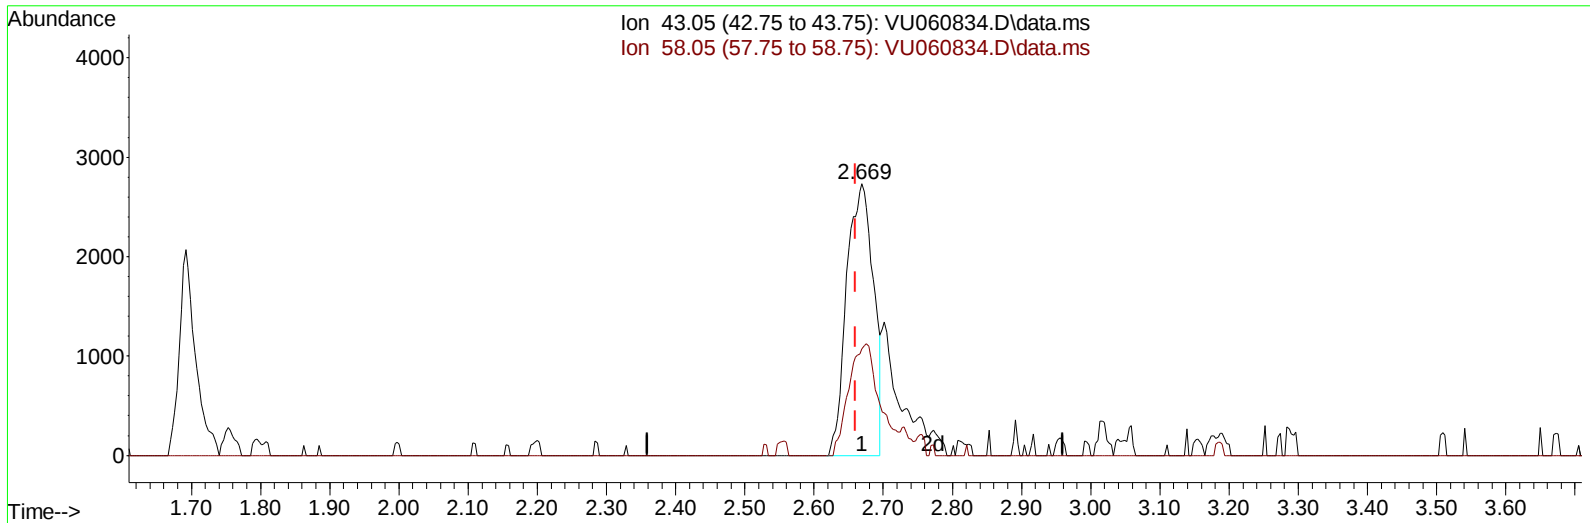

TIC: VU060834.D\data.ms

(13) Acetone (T)

2.669min (+ 0.010) 5.35 ug/L

response 7343

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.80	47.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091724\
Data File : VU060834.D
Acq On : 17 Sep 2024 15:42
Operator : MD/SY
Sample : P3973-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT2

Manual IntegrationsAPPROVED

Quant Time: Sep 18 01:18:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 18 01:15:55 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/18/2024
Supervised By :Semsettin Yesilyurt 09/18/2024

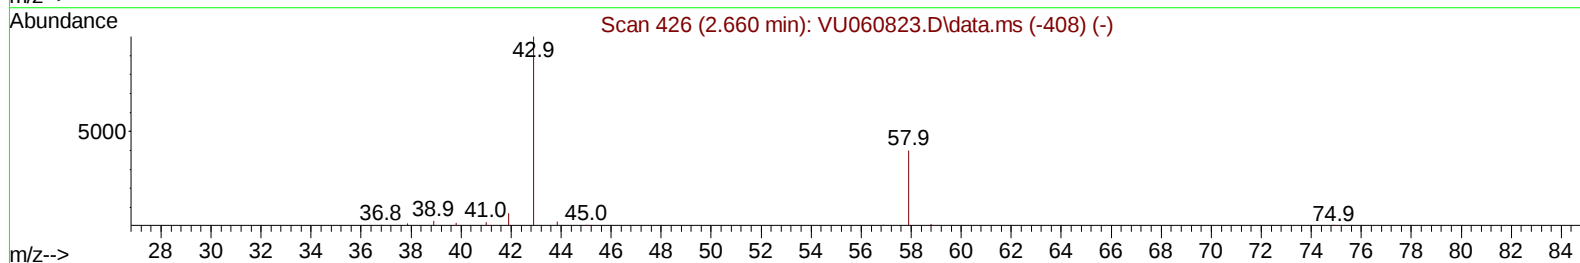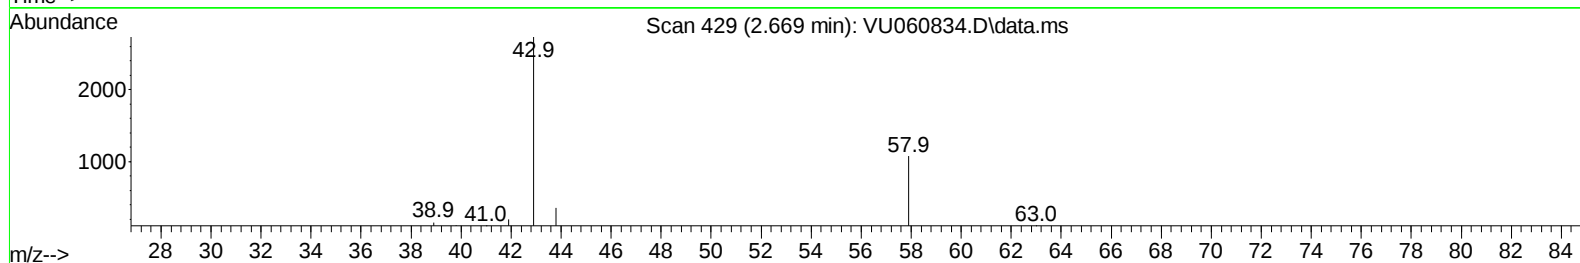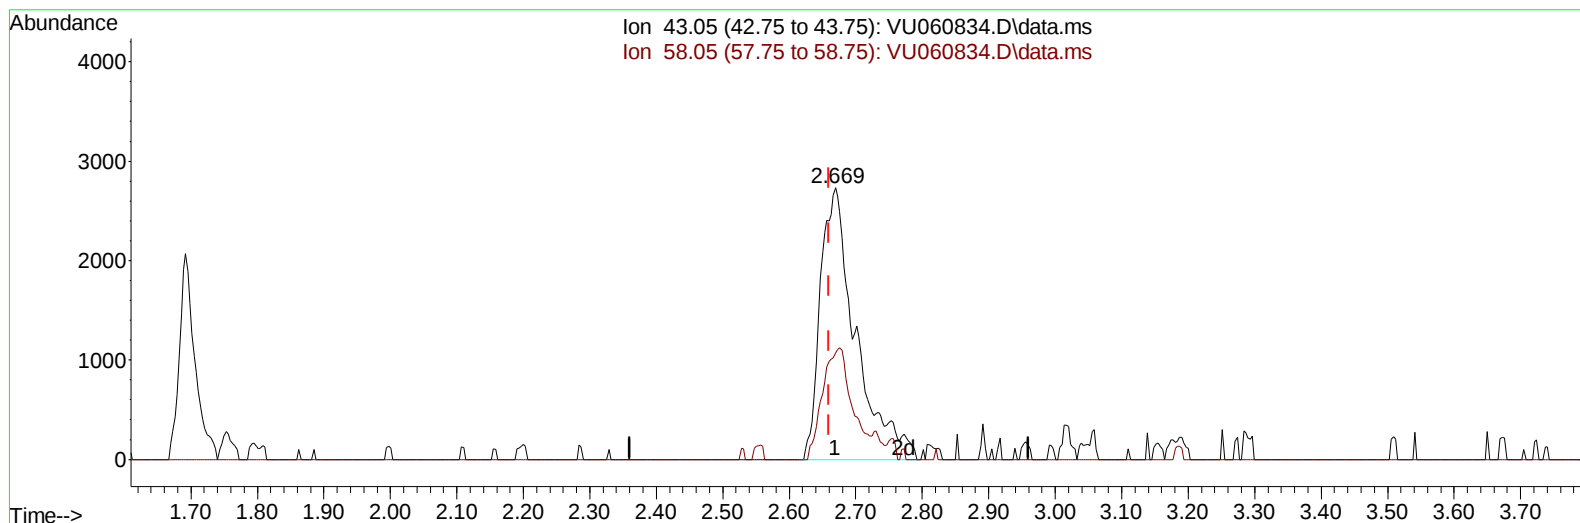

TIC: VU060834.D\data.ms

(13) Acetone (T)

2.669min (+ 0.010) 7.32 ug/L m

response 10051

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.80	34.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091724\
 Data File : VU060834.D
 Acq On : 17 Sep 2024 15:42
 Operator : MD/SY
 Sample : P3973-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AT2

Manual IntegrationsAPPROVED

Quant Time: Sep 18 01:18:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 18 01:15:55 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/18/2024
 Supervised By :Semsettin Yesilyurt 09/18/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		142593	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		152437	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		60145	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		51268	3.997	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	80.000%		
7) Chloroethane-d5	1.911	69		40213	4.404	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	88.000%		
11) 1,1-Dichloroethene-d2	2.563	65		21547	4.740	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	94.800%		
20) 2-Butanone-d5	4.637	46		98085	47.639	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	95.280%		
24) Chloroform-d	5.052	84		89717	4.576	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	91.600%		
26) 1,2-Dichloroethane-d4	5.695	65		45079	4.810	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	96.200%		
32) Benzene-d6	5.721	84		179738	4.399	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	88.000%		
36) 1,2-Dichloropropane-d6	6.682	67		58389	4.619	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	92.400%		
41) Toluene-d8	7.891	98		149410	4.011	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	80.200%		
43) trans-1,3-Dichloroprop...	8.177	79		19978	4.390	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	87.800%		
46) 2-Hexanone-d5	8.631	63		77757	43.320	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	86.640%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84		45774	4.622	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	92.400%		
66) 1,2-Dichlorobenzene-d4	12.187	152		52557	5.200	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	104.000%		
Target Compounds							
						Qvalue	
13) Acetone	2.669	43		10051m	7.317	ug/L	
14) Carbon disulfide	2.788	76		15019	0.604	ug/L	99
16) Methylene chloride	3.039	84		2584	0.249	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091724\
Data File : VU060834.D
Acq On : 17 Sep 2024 15:42
Operator : MD/SY
Sample : P3973-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT2

Manual IntegrationsAPPROVED

Quant Time: Sep 18 01:18:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 18 01:15:55 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/18/2024
Supervised By :Semsettin Yesilyurt 09/18/2024

