

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091724\
 Data File : VU060836.D
 Acq On : 17 Sep 2024 16:31
 Operator : MD/SY
 Sample : P3973-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AW5

Quant Time: Sep 18 01:19:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 18 01:15:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	142873	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	153137	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	59343	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	49667	3.865	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.200%	
7) Chloroethane-d5	1.911	69	38883	4.250	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.000%	
11) 1,1-Dichloroethene-d2	2.563	65	18560	4.075	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	81.400%	
20) 2-Butanone-d5	4.637	46	89634	43.449	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	86.900%	
24) Chloroform-d	5.055	84	85327	4.343	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.800%	
26) 1,2-Dichloroethane-d4	5.695	65	41015	4.368	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.400%	
32) Benzene-d6	5.721	84	165027	4.021	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.400%	
36) 1,2-Dichloropropane-d6	6.682	67	54745	4.311	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	86.200%	
41) Toluene-d8	7.891	98	136993	3.661	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	73.200%	
43) trans-1,3-Dichloroprop...	8.174	79	17267	3.777	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	75.600%	
46) 2-Hexanone-d5	8.631	63	69925	38.778	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	77.560%	
56) 1,1,2,2-Tetrachloroeth...	10.746	84	41654	4.187	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	83.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152	49931	5.007	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.200%	
Target Compounds					Qvalue	
13) Acetone	2.660	43	19931	14.481	ug/L	99
14) Carbon disulfide	2.792	76	14199	0.570	ug/L	98
42) Toluene	7.968	91	15957	0.362	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091724\
Data File : VU060836.D
Acq On : 17 Sep 2024 16:31
Operator : MD/SY
Sample : P3973-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AW5

Quant Time: Sep 18 01:19:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 18 01:15:55 2024
Response via : Initial Calibration

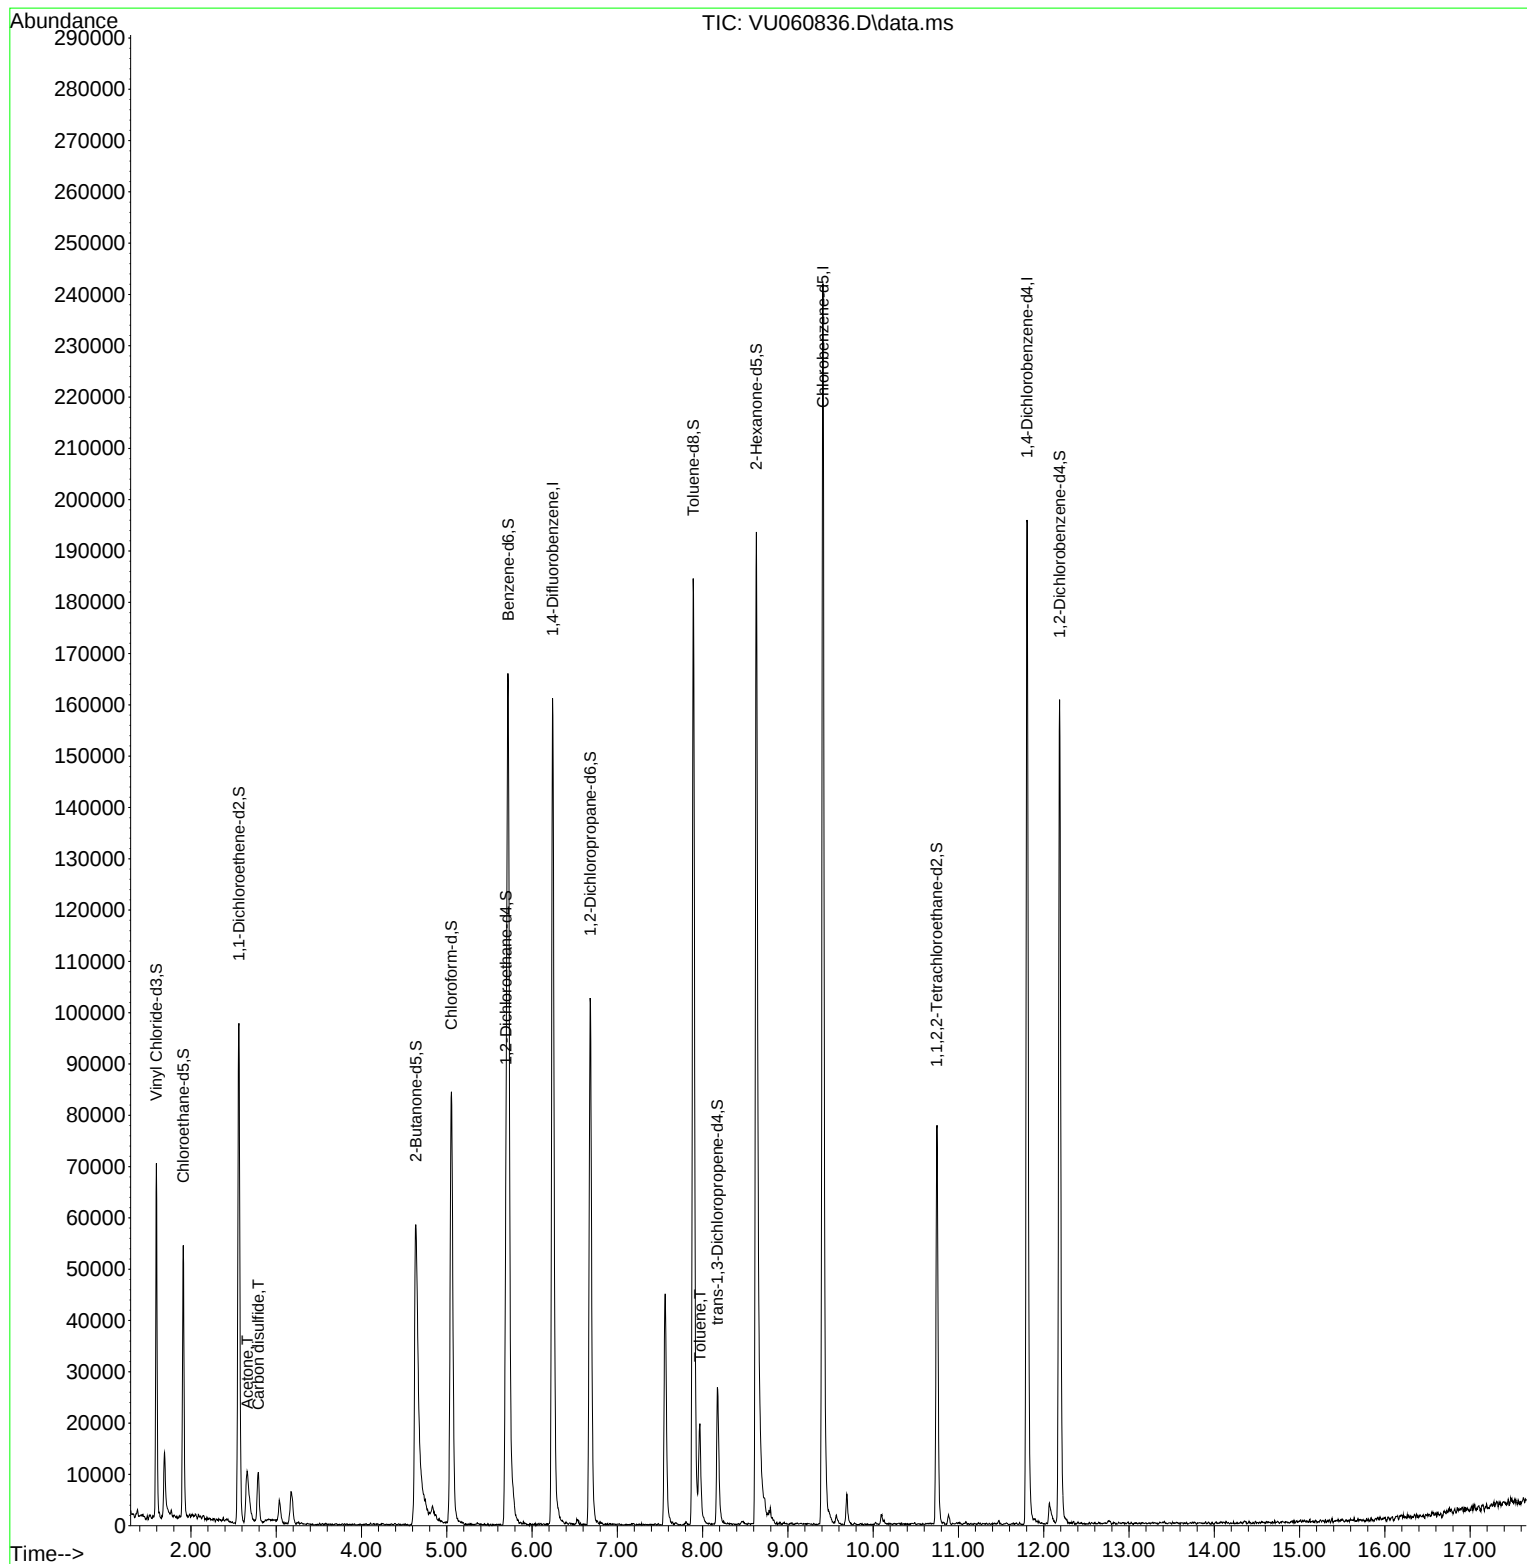

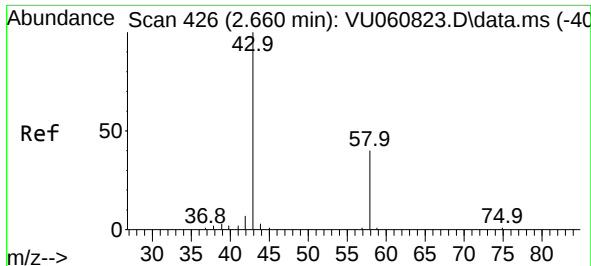

#13

Acetone

Concen: 14.481 ug/L

RT: 2.660 min Scan# 41

Delta R.T. 0.000 min

Lab File: VU060836.D

Acq: 17 Sep 2024 16:31

Instrument :

MSVOA_U

ClientSampleId :





C0AW5

Tgt Ion: 43 Resp: 19931

Ion Ratio Lower Upper

43 100

58 35.4 0.0 69.6

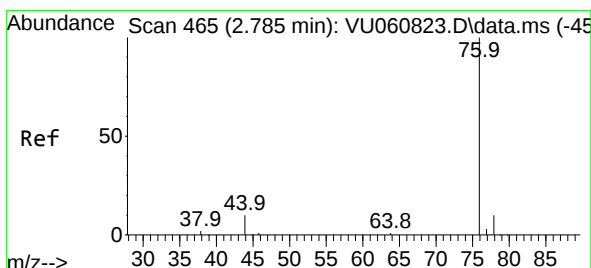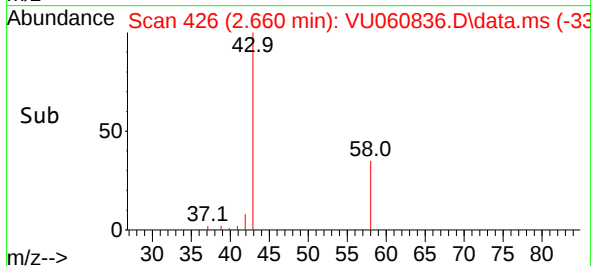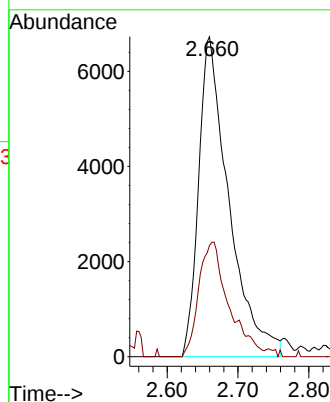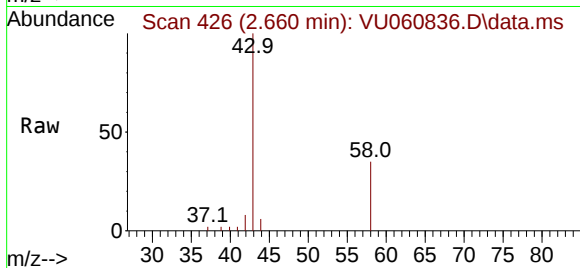

#14

Carbon disulfide

Concen: 0.570 ug/L

RT: 2.792 min Scan# 467

Delta R.T. 0.006 min

Lab File: VU060836.D




Acq: 17 Sep 2024 16:31


Tgt Ion: 76 Resp: 14199

Ion Ratio Lower Upper

76 100

78 9.8 7.1 10.7

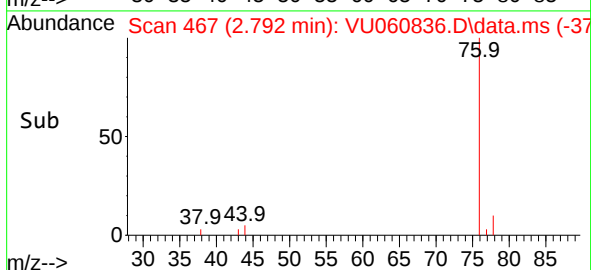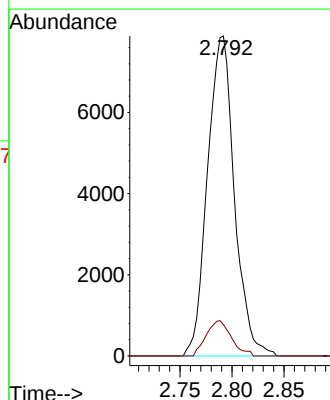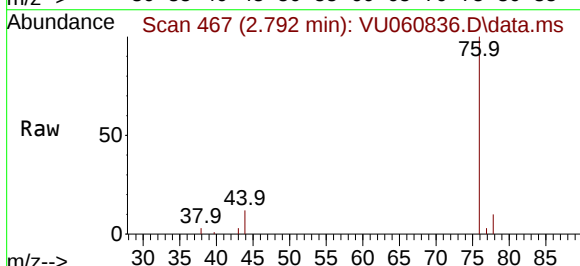

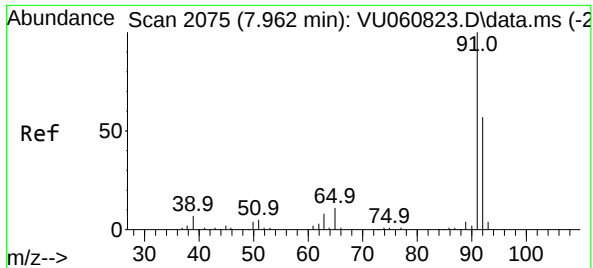

#42

Toluene

Concen: 0.362 ug/L

RT: 7.968 min Scan# 20

Delta R.T. 0.006 min

Lab File: VU060836.D


Acq: 17 Sep 2024 16:31

Instrument :

MSVOA_U

ClientSampleId :

C0AW5

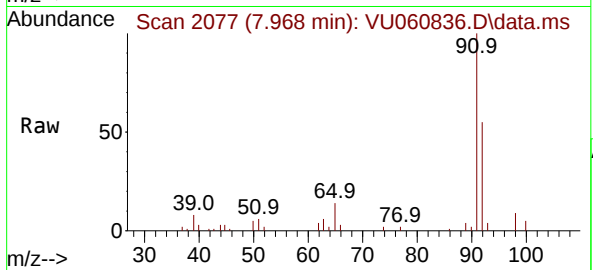

Tgt Ion: 91 Resp: 15957

Ion Ratio Lower Upper

91 100

92 55.3 40.5 75.3

