


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091724\
Data File : VU060822.D
Acq On : 17 Sep 2024 09:38
Operator : MD/SY
Sample : BFB198
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB198

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 19 05:11:13 2024

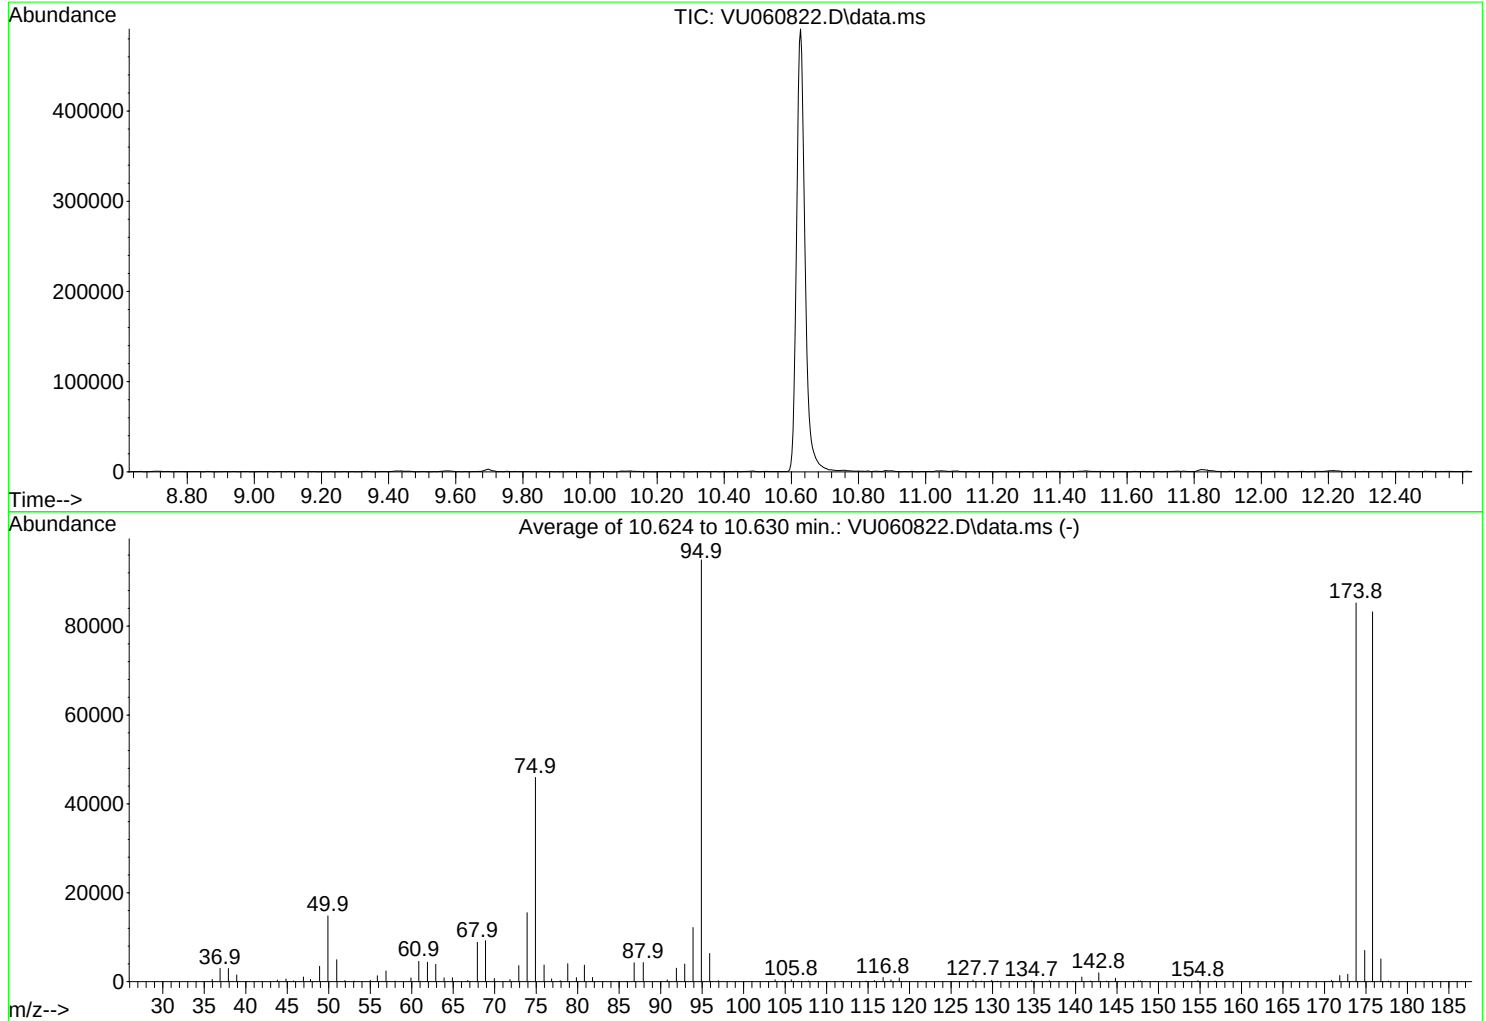

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	14795	PASS
75	95	30	80	48.4	45963	PASS
95	95	100	100	100.0	94920	PASS
96	95	5	9	6.7	6356	PASS
173	174	0.00	2	1.9	1651	PASS
174	95	50	120	89.8	85229	PASS
175	174	5	9	8.3	7041	PASS
176	174	95	101	97.6	83197	PASS
177	176	5	9	6.1	5101	PASS

m/z	Abundance
43.80	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198

m/z	Abundance
36.00	590.0
36.90	3110.0
37.90	2883.0
38.90	1571.0
40.10	104.0
43.80	596.0
44.80	666.0
45.80	153.0
46.90	995.0
47.80	516.0
48.90	3374.0
49.90	15189.0
50.90	4910.0
52.00	210.0
53.00	131.0
55.00	298.0
55.80	1273.0
56.90	2391.0
58.00	207.0
59.90	853.0
60.80	4457.0
61.90	4724.0
62.90	4131.0
63.90	786.0
64.90	790.0
66.80	307.0
67.90	8454.0
68.90	9418.0
69.90	667.0
71.90	486.0
72.90	3606.0
73.90	15724.0
74.90	46040.0
76.00	3799.0
76.80	650.0
77.90	289.0
78.80	3836.0
79.90	859.0
80.80	3835.0
81.80	929.0
86.80	4182.0
87.90	4201.0
90.80	411.0
91.90	3308.0
92.90	4190.0
93.90	12169.0
94.90	96448.0
95.90	6262.0
97.00	205.0
103.80	433.0
104.70	215.0
105.70	443.0
106.60	122.0
107.70	126.0
111.80	123.0
114.70	150.0
115.70	221.0
116.80	982.0
117.80	408.0
118.70	814.0
127.60	397.0
128.60	136.0
129.90	271.0
134.70	227.0
136.90	204.0
139.70	117.0
140.80	1117.0
141.80	108.0
142.80	1848.0
143.80	179.0
144.80	831.0
147.60	225.0
147.90	223.0
149.60	131.0
154.70	340.0
156.80	182.0
170.80	312.0
171.80	1297.0
172.80	1625.0
173.80	83552.0
174.80	6906.0
175.80	81456.0
176.80	4891.0
177.80	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198

m/z	Abundance
36.00	499.0
36.90	3039.0
37.90	3045.0
38.90	1585.0
43.80	633.0
44.90	610.0
45.70	152.0
46.90	1106.0
47.80	507.0
48.90	3591.0
49.90	15279.0
51.00	5108.0
52.00	267.0
53.10	139.0
55.00	309.0
55.80	1393.0
56.90	2447.0
58.00	161.0
59.90	897.0
60.90	4827.0
61.90	4383.0
62.90	3947.0
63.90	953.0
64.90	882.0
66.80	269.0
67.90	9145.0
68.90	9465.0
70.00	738.0
71.90	526.0
72.90	3677.0
73.90	15992.0
74.90	47184.0
75.90	3835.0
76.90	643.0
78.80	4161.0
79.80	955.0
80.80	3869.0
81.80	993.0
86.80	4338.0
87.90	4422.0
90.80	373.0
91.90	3104.0
92.90	4064.0
93.90	12583.0
94.90	97760.0
95.90	6585.0
96.90	228.0
103.80	438.0
104.70	170.0
105.80	462.0
106.60	124.0
107.80	140.0
111.80	121.0
114.80	178.0
115.70	255.0
116.80	965.0
117.70	395.0
118.80	895.0
127.60	383.0
128.70	129.0
129.90	270.0
130.60	134.0
134.70	248.0
136.80	231.0
139.70	107.0
140.70	1070.0
141.80	159.0
142.80	2026.0
143.80	149.0
144.80	791.0
147.60	280.0
149.60	130.0
154.80	238.0
156.80	176.0
170.80	310.0
171.90	1422.0
172.80	1695.0
173.80	87824.0
174.80	7298.0
175.80	85592.0
176.80	5235.0
177.70	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198

m/z	Abundance
35.80	413.0
36.90	2820.0
37.90	2981.0
38.90	1418.0
43.80	663.0
44.90	528.0
45.60	118.0
45.90	117.0
47.00	1059.0
47.80	471.0
48.90	3430.0
49.90	13916.0
50.90	4770.0
51.90	257.0
53.10	156.0
55.00	229.0
55.90	1309.0
56.90	2443.0
58.00	107.0
59.90	841.0
60.90	4473.0
61.90	3927.0
62.90	3542.0
63.90	895.0
64.90	898.0
66.70	259.0
67.90	8953.0
68.90	8788.0
70.00	795.0
71.80	434.0
72.90	3568.0
73.90	14805.0
74.90	44664.0
75.90	3591.0
76.90	556.0
77.90	374.0
78.80	4099.0
79.80	936.0
80.80	3460.0
81.80	941.0
85.90	181.0
86.80	4203.0
87.90	4196.0
90.80	367.0
91.90	2652.0
92.90	3594.0
93.90	11744.0
94.90	90552.0
95.90	6222.0
96.90	218.0
103.80	400.0
105.00	150.0
105.80	402.0
107.90	141.0
109.90	102.0
114.80	153.0
115.80	297.0
116.80	911.0
117.70	408.0
118.80	811.0
127.70	324.0
128.70	134.0
129.90	334.0
130.60	160.0
134.70	194.0
136.80	201.0
139.70	101.0
140.70	996.0
141.80	179.0
142.80	2087.0
143.70	128.0
144.80	720.0
147.80	319.0
154.80	194.0
156.70	114.0
158.60	108.0
170.90	266.0
171.90	1347.0
172.80	1633.0
173.80	84312.0
174.90	6920.0
175.80	82544.0
176.80	5177.0
177.80	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB198