
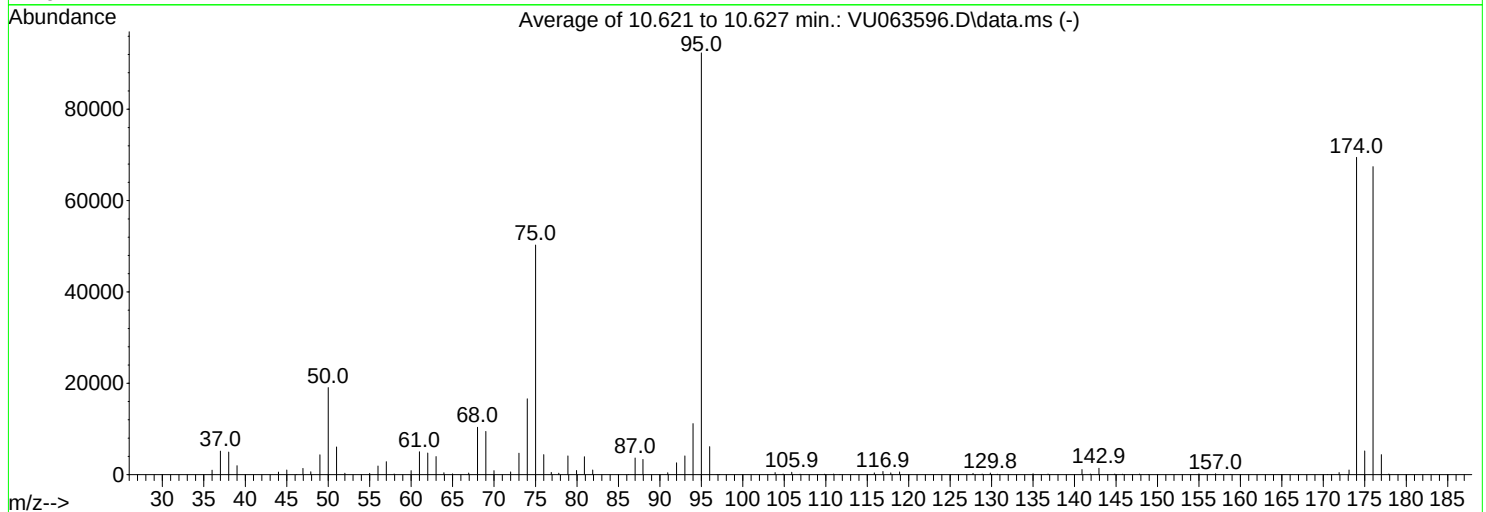


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091725\
Data File : VU063596.D
Acq On : 17 Sep 2025 08:22
Operator : MD/SY
Sample : BFB084
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB084

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091725WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Sep 19 06:13:08 2025

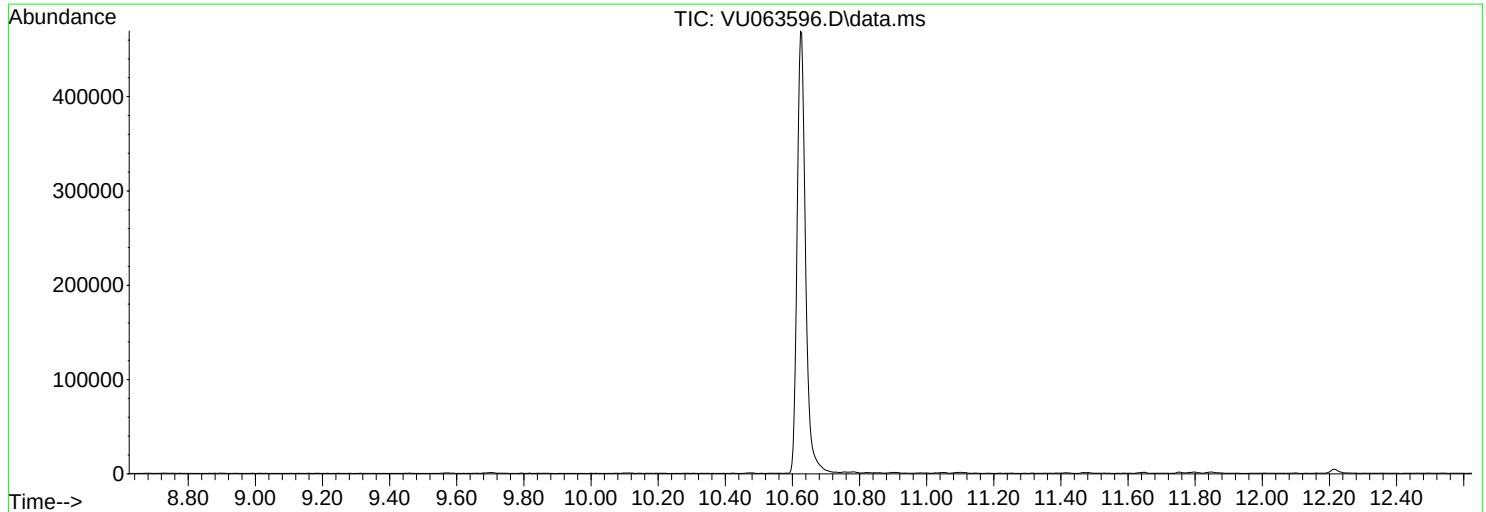

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	19061	PASS
75	95	30	80	54.4	50269	PASS
95	95	100	100	100.0	92357	PASS
96	95	5	9	6.7	6151	PASS
173	174	0.00	2	1.4	1000	PASS
174	95	50	120	75.2	69459	PASS
175	174	5	9	7.5	5188	PASS
176	174	95	101	97.1	67432	PASS
177	176	5	9	6.5	4372	PASS

m/z	Abundance
39.90	239.0
44.00	571.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
36.00	972.0
37.00	5024.0
38.00	4656.0
39.00	1933.0
39.90	228.0
44.00	1175.0
45.00	863.0
46.90	1206.0
47.90	636.0
49.00	4204.0
50.00	18224.0
51.00	5932.0
52.00	277.0
55.00	229.0
56.00	1844.0
57.00	2715.0
58.10	112.0
60.00	852.0
61.00	4774.0
62.00	4453.0
63.00	3884.0
63.90	417.0
65.10	183.0
66.90	318.0
68.00	10117.0
69.00	9123.0
70.00	808.0
72.00	538.0
73.00	4344.0
74.00	15784.0
75.00	48168.0
76.00	4189.0
76.90	418.0
77.80	302.0
78.90	4046.0
80.00	909.0
80.90	3822.0
81.90	979.0
87.00	3259.0
87.90	3094.0
91.00	420.0
92.00	2535.0
93.00	3794.0
94.00	11060.0
95.00	88192.0
96.00	5923.0
103.90	415.0
104.90	116.0
105.90	482.0
106.90	107.0
109.90	100.0
111.00	112.0
111.70	113.0
115.80	404.0
116.90	733.0
117.90	353.0
118.90	591.0
127.70	237.0
128.80	160.0
129.90	357.0
135.00	152.0
136.80	179.0
140.90	1138.0
141.90	140.0
142.90	1280.0
144.90	144.0
145.80	173.0
147.80	155.0
148.90	107.0
155.00	159.0
157.00	197.0
171.90	414.0
173.10	899.0
174.00	64264.0
175.00	4903.0
176.00	62624.0
177.00	4072.0
177.90	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
36.00	1017.0
37.00	5255.0
38.00	5067.0
39.00	2061.0
39.90	247.0
44.00	1214.0
45.00	1053.0
46.20	106.0
46.90	1464.0
47.90	646.0
49.00	4487.0
50.00	19704.0
51.00	6273.0
52.00	331.0
55.00	305.0
56.00	1949.0
57.00	2905.0
57.90	129.0
60.00	890.0
61.00	5204.0
62.00	4846.0
63.00	4091.0
63.90	434.0
65.00	174.0
66.90	367.0
68.00	10711.0
69.00	9612.0
70.00	914.0
72.00	608.0
73.00	4791.0
74.00	17040.0
75.00	51832.0
76.00	4527.0
76.90	499.0
77.80	314.0
78.90	4200.0
80.00	945.0
80.90	4020.0
81.90	1065.0
87.00	3686.0
88.00	3346.0
91.00	421.0
92.00	2665.0
93.00	4161.0
94.00	11515.0
95.00	95400.0
96.00	6383.0
103.90	454.0
104.80	153.0
105.90	546.0
106.90	123.0
109.90	101.0
111.00	160.0
115.80	377.0
116.90	704.0
117.80	392.0
118.90	637.0
127.70	292.0
128.80	163.0
129.80	331.0
130.70	117.0
135.00	225.0
136.80	162.0
140.90	1132.0
141.90	160.0
142.90	1436.0
144.90	143.0
145.80	167.0
147.80	125.0
155.00	169.0
157.00	233.0
158.90	118.0
171.90	474.0
173.10	1051.0
174.00	71352.0
175.00	5328.0
176.00	69160.0
177.00	4534.0
177.90	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
36.00	937.0
37.00	5176.0
38.00	5092.0
39.00	1898.0
39.90	227.0
44.00	1042.0
45.00	1133.0
47.00	1405.0
47.90	591.0
49.00	4381.0
50.00	19256.0
51.00	5951.0
52.00	320.0
55.00	350.0
56.00	1883.0
57.00	2895.0
57.90	159.0
60.00	878.0
61.00	5014.0
62.00	4886.0
63.00	3955.0
64.00	421.0
64.90	178.0
67.00	346.0
68.00	10340.0
69.00	9623.0
70.00	956.0
72.00	598.0
73.00	4908.0
74.00	17056.0
75.00	50808.0
76.00	4378.0
76.90	520.0
77.80	317.0
78.90	4006.0
79.90	905.0
80.90	3891.0
81.90	980.0
86.20	101.0
87.00	3955.0
88.00	3565.0
90.90	429.0
92.00	2558.0
93.00	4302.0
94.00	10930.0
95.00	93480.0
96.00	6146.0
96.90	129.0
97.20	136.0
103.90	465.0
104.90	185.0
105.90	520.0
106.90	120.0
109.80	108.0
110.90	178.0
115.90	343.0
116.90	653.0
117.80	394.0
118.90	592.0
127.80	343.0
128.90	134.0
129.80	334.0
130.70	166.0
135.00	274.0
136.80	117.0
140.90	1064.0
141.90	152.0
143.00	1455.0
144.80	121.0
146.00	152.0
147.90	120.0
155.00	153.0
157.00	254.0
158.80	144.0
170.50	100.0
171.00	114.0
171.90	524.0
173.10	1051.0
174.00	72760.0
175.00	5334.0
176.00	70512.0
177.00	4510.0
177.90	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084