

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091818\
 Data File : VU026847.D
 Acq On : 18 Sep 2018 09:26
 Operator : MD/SY
 Sample : J4893-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	63	69	85	rVB	132118	139413	14.27%	1.977%
2	1.678	149	157	179	rVB	105217	138761	14.20%	1.968%
3	2.273	331	342	355	rBV	221825	335117	34.30%	4.753%
4	2.549	426	428	429	rBV	236	94	0.01%	0.001%
5	2.884	529	532	535	rVB	133	63	0.01%	0.001%
6	2.951	551	553	555	rVB	119	47	0.00%	0.001%
7	3.000	566	568	569	rBV	165	68	0.01%	0.001%
8	3.041	577	581	586	rVB2	252	221	0.02%	0.003%
9	3.096	596	598	600	rBV	168	59	0.01%	0.001%
10	3.125	605	607	609	rBV	148	107	0.01%	0.002%
11	3.170	618	621	625	rVB	175	109	0.01%	0.002%
12	3.189	625	627	631	rBV	173	131	0.01%	0.002%
13	3.273	651	653	654	rBV	136	36	0.00%	0.001%
14	3.295	659	660	661	rBV	120	30	0.00%	0.000%
15	3.356	676	679	684	rBV	106	94	0.01%	0.001%
16	3.382	684	687	688	rBV	226	151	0.02%	0.002%
17	3.440	700	705	708	rBV2	181	185	0.02%	0.003%
18	3.572	744	746	748	rBV2	153	101	0.01%	0.001%
19	3.620	758	761	764	rBV	111	74	0.01%	0.001%
20	3.662	772	774	777	rBV	90	57	0.01%	0.001%
21	3.774	806	809	812	rVB	146	89	0.01%	0.001%
22	3.906	848	850	852	rBV	163	71	0.01%	0.001%
23	4.176	919	934	963	rBV	78778	212002	21.70%	3.007%
24	4.450	1018	1019	1026	rVB2	139	146	0.01%	0.002%
25	4.504	1034	1036	1038	rBV	158	50	0.01%	0.001%
26	4.540	1046	1047	1048	rVB	107	21	0.00%	0.000%
27	4.649	1062	1081	1108	rBV	165526	385966	39.50%	5.474%
28	4.877	1149	1152	1155	rBV2	288	257	0.03%	0.004%
29	4.948	1171	1174	1175	rBV	182	76	0.01%	0.001%
30	4.974	1181	1182	1187	rVB	146	52	0.01%	0.001%
31	4.996	1187	1189	1190	rBV	111	44	0.00%	0.001%
32	5.032	1194	1200	1201	rBV2	201	151	0.02%	0.002%
33	5.080	1213	1215	1218	rVB	141	39	0.00%	0.001%
34	5.160	1239	1240	1241	rBV	106	24	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091818\
 Data File : VU026847.D
 Acq On : 18 Sep 2018 09:26
 Operator : MD/SY
 Sample : J4893-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

35	5.170	1241	1243	1244	rBV	74	30	0.00%	0.000%
36	5.244	1261	1266	1271	rBV	105	152	0.02%	0.002%
37	5.340	1271	1296	1328	rVV2	334554	977149	100.00%	13.859%
38	5.562	1363	1365	1368	rVB	183	84	0.01%	0.001%
39	5.581	1368	1371	1374	rBV	66	40	0.00%	0.001%
40	5.601	1374	1377	1380	rBV	126	80	0.01%	0.001%
41	5.652	1390	1393	1395	rBV	192	117	0.01%	0.002%
42	5.672	1398	1399	1400	rVB	99	21	0.00%	0.000%
43	5.720	1410	1414	1418	rVB	87	66	0.01%	0.001%
44	5.755	1420	1425	1429	rBV2	179	179	0.02%	0.003%
45	5.887	1450	1466	1487	rBV	292581	567234	58.05%	8.045%
46	6.073	1522	1524	1528	rVB	146	102	0.01%	0.001%
47	6.096	1528	1531	1534	rVB	72	38	0.00%	0.001%
48	6.118	1536	1538	1540	rVB	141	55	0.01%	0.001%
49	6.135	1540	1543	1545	rBV	59	36	0.00%	0.001%
50	6.231	1572	1573	1574	rBV	87	20	0.00%	0.000%
51	6.331	1590	1604	1629	rBV	223196	446938	45.74%	6.339%
52	6.453	1637	1642	1645	rBV3	249	190	0.02%	0.003%
53	6.527	1664	1665	1669	rVB	156	56	0.01%	0.001%
54	6.594	1684	1686	1687	rVV	100	22	0.00%	0.000%
55	6.607	1688	1690	1696	rVB2	175	137	0.01%	0.002%
56	6.668	1707	1709	1712	rVB	161	71	0.01%	0.001%
57	6.710	1719	1722	1727	rVB	165	104	0.01%	0.001%
58	6.803	1749	1751	1752	rBV	137	60	0.01%	0.001%
59	6.855	1763	1767	1770	rBV	478	437	0.04%	0.006%
60	6.897	1779	1780	1781	rVB	103	20	0.00%	0.000%
61	6.983	1806	1807	1808	rBV	109	23	0.00%	0.000%
62	7.089	1838	1840	1842	rBV	149	40	0.00%	0.001%
63	7.144	1855	1857	1860	rBV	127	57	0.01%	0.001%
64	7.228	1871	1883	1906	rBV	109414	193792	19.83%	2.749%
65	7.337	1913	1917	1920	rVB	298	123	0.01%	0.002%
66	7.356	1921	1923	1925	rVB	139	57	0.01%	0.001%
67	7.379	1927	1930	1931	rBV	205	131	0.01%	0.002%
68	7.450	1949	1952	1955	rBV	45	34	0.00%	0.000%
69	7.469	1955	1958	1961	rVB2	152	86	0.01%	0.001%
70	7.482	1961	1962	1963	rBV2	212	47	0.00%	0.001%
71	7.565	1975	1988	2009	rBV	431598	743208	76.06%	10.541%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091818\
 Data File : VU026847.D
 Acq On : 18 Sep 2018 09:26
 Operator : MD/SY
 Sample : J4893-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

72	7.720	2032	2036	2043	rBV3	590	855	0.09%	0.012%
73	7.848	2065	2076	2094	rBV	77744	131876	13.50%	1.870%
74	8.060	2140	2142	2144	rVB	157	44	0.00%	0.001%
75	8.077	2144	2147	2150	rBV2	207	176	0.02%	0.002%
76	8.096	2150	2153	2155	rVV2	186	111	0.01%	0.002%
77	8.134	2163	2165	2168	rBV	156	93	0.01%	0.001%
78	8.311	2209	2220	2249	rBV	248922	426926	43.69%	6.055%
79	8.562	2296	2298	2301	rBB2	244	131	0.01%	0.002%
80	8.617	2309	2315	2325	rVB3	1118	2056	0.21%	0.029%
81	8.675	2332	2333	2335	rBV2	224	104	0.01%	0.001%
82	8.700	2340	2341	2343	rBV	157	57	0.01%	0.001%
83	8.713	2343	2345	2348	rVB	159	56	0.01%	0.001%
84	8.945	2415	2417	2420	rBV	174	108	0.01%	0.002%
85	9.089	2449	2462	2486	rBV	416254	679527	69.54%	9.638%
86	9.302	2524	2528	2533	rBV2	306	242	0.02%	0.003%
87	9.340	2538	2540	2544	rVB2	375	232	0.02%	0.003%
88	9.437	2566	2570	2572	rBV	164	143	0.01%	0.002%
89	9.514	2589	2594	2600	rBV2	286	373	0.04%	0.005%
90	9.572	2609	2612	2614	rBV	290	160	0.02%	0.002%
91	9.678	2641	2645	2649	rBV	198	177	0.02%	0.003%
92	10.128	2781	2785	2787	rBV2	198	158	0.02%	0.002%
93	10.163	2791	2796	2798	rBV2	333	239	0.02%	0.003%
94	10.327	2844	2847	2850	rBV	230	123	0.01%	0.002%
95	10.433	2868	2880	2896	rBV	292622	464369	47.52%	6.586%
96	11.176	3108	3111	3114	rBV	275	174	0.02%	0.002%
97	11.485	3195	3207	3228	rBV	353823	558775	57.18%	7.925%
98	11.861	3311	3324	3345	rBV	404696	638235	65.32%	9.052%


Sum of corrected areas: 7050462

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091818\
Data File : VU026847.D
Acq On : 18 Sep 2018 09:26
Operator : MD/SY
Sample : J4893-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

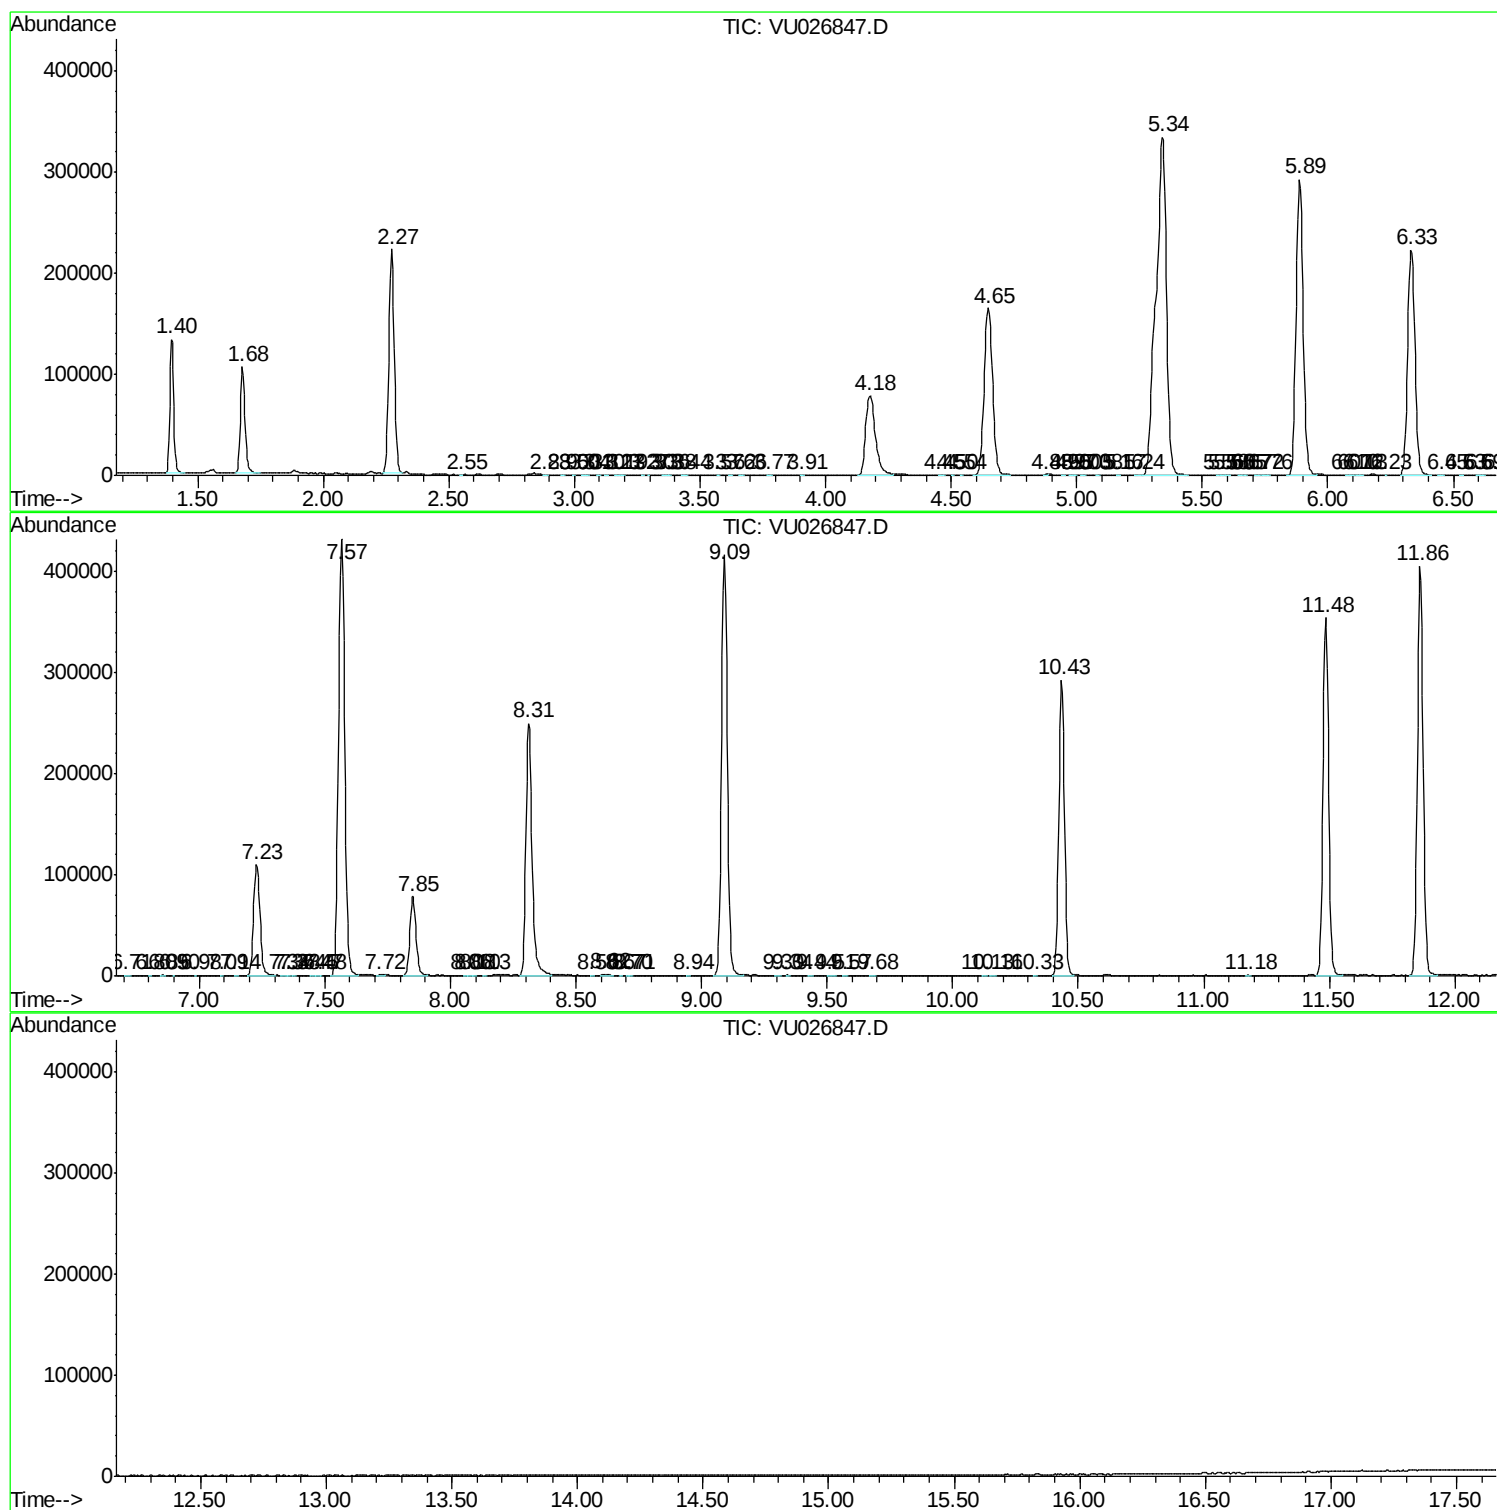

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091818\
Data File : VU026847.D
Acq On : 18 Sep 2018 09:26
Operator : MD/SY
Sample : J4893-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091818\
Data File : VU026847.D
Acq On : 18 Sep 2018 09:26
Operator : MD/SY
Sample : J4893-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc