


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091818\
Data File : VU026843.D
Acq On : 18 Sep 2018 07:25
Operator : MD/SY
Sample : BFB41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Title : VOC Analysis
Last Update : Fri Sep 21 04:24:07 2018

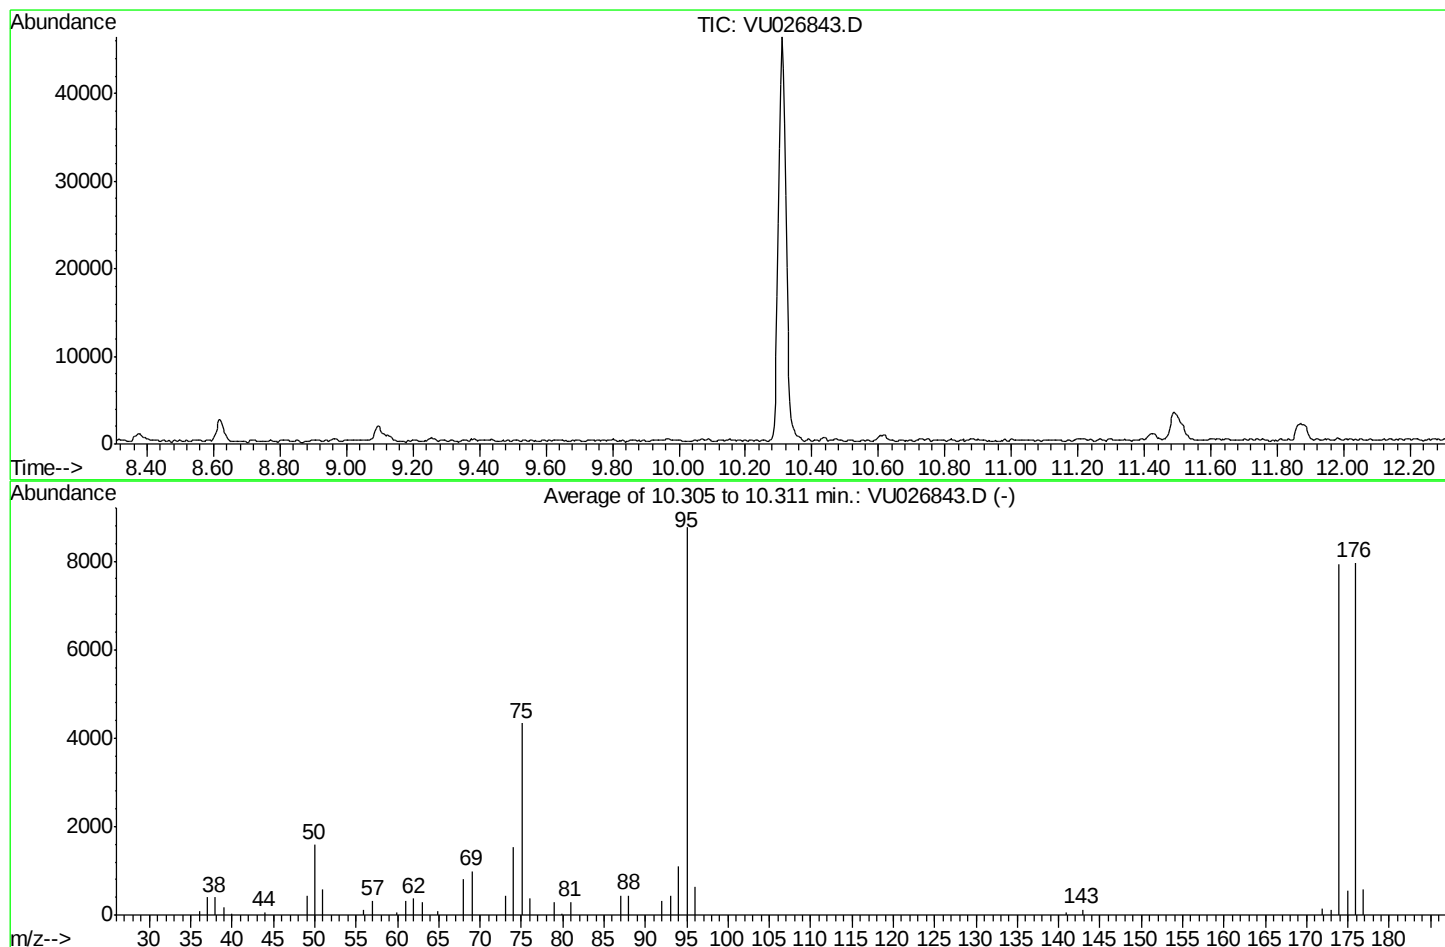

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	1587	PASS
75	95	30	80	49.4	4333	PASS
95	95	100	100	100.0	8767	PASS
96	95	5	9	7.2	627	PASS
173	174	0.00	2	1.6	124	PASS
174	95	50	120	90.6	7942	PASS
175	174	5	9	6.8	540	PASS
176	174	95	101	100.3	7967	PASS
177	176	5	9	7.2	570	PASS

Scan 2830 (10.273 min): VU026843.D
BFB41

m/z	Abundance
39.90	136.0
43.90	325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.90	372.0
37.90	377.0
39.10	177.0
40.00	148.0
44.00	394.0
49.00	357.0
50.00	1494.0
51.00	493.0
55.90	118.0
57.00	346.0
61.00	304.0
62.00	348.0
63.00	229.0
68.00	780.0
69.10	905.0
73.00	404.0
74.00	1466.0
75.10	4034.0
76.00	339.0
78.90	240.0
80.90	273.0
86.90	426.0
88.00	402.0
92.00	297.0
93.10	452.0
94.00	962.0
95.10	8351.0
96.00	618.0
142.90	101.0
171.90	149.0
172.90	118.0
174.00	7334.0
175.00	493.0
175.90	7140.0
176.90	563.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	118.0
37.00	414.0
37.90	422.0
39.00	191.0
40.00	155.0
44.00	372.0
49.00	447.0
50.00	1614.0
51.00	589.0
55.90	119.0
57.00	349.0
59.90	100.0
61.00	307.0
62.00	377.0
63.00	297.0
64.90	103.0
68.00	837.0
69.00	1043.0
73.00	457.0
74.00	1582.0
75.10	4440.0
76.00	396.0
78.90	298.0
79.90	105.0
80.90	305.0
87.00	434.0
88.00	465.0
92.00	352.0
93.10	435.0
94.10	1135.0
95.10	9001.0
96.00	639.0
140.90	107.0
142.90	119.0
171.90	143.0
172.90	125.0
174.00	8187.0
174.90	538.0
175.90	8269.0
176.90	588.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	128.0
37.10	417.0
37.90	407.0
39.00	191.0
39.90	157.0
44.00	394.0
49.00	496.0
50.00	1653.0
51.00	640.0
55.90	126.0
57.00	304.0
59.90	106.0
60.90	318.0
61.90	389.0
63.00	326.0
64.90	123.0
68.00	810.0
69.00	1017.0
73.00	437.0
74.00	1584.0
75.00	4525.0
76.00	400.0
78.90	339.0
80.90	293.0
87.00	438.0
88.00	460.0
92.00	326.0
93.00	387.0
94.10	1210.0
95.00	8950.0
96.00	624.0
140.90	113.0
142.90	150.0
172.00	133.0
173.00	131.0
173.90	8306.0
174.90	590.0
175.90	8493.0
176.90	559.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41