


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091820\
Data File : VU040220.D
Acq On : 18 Sep 2020 18:45
Operator : SY/MD
Sample : L4078-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK9

Manual Integrations
APPROVED

MMDadoda
9/21/2020 1:38:14 PM

Quant Time: Sep 19 01:06:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Sep 18 23:20:35 2020
Response via : Initial Calibration

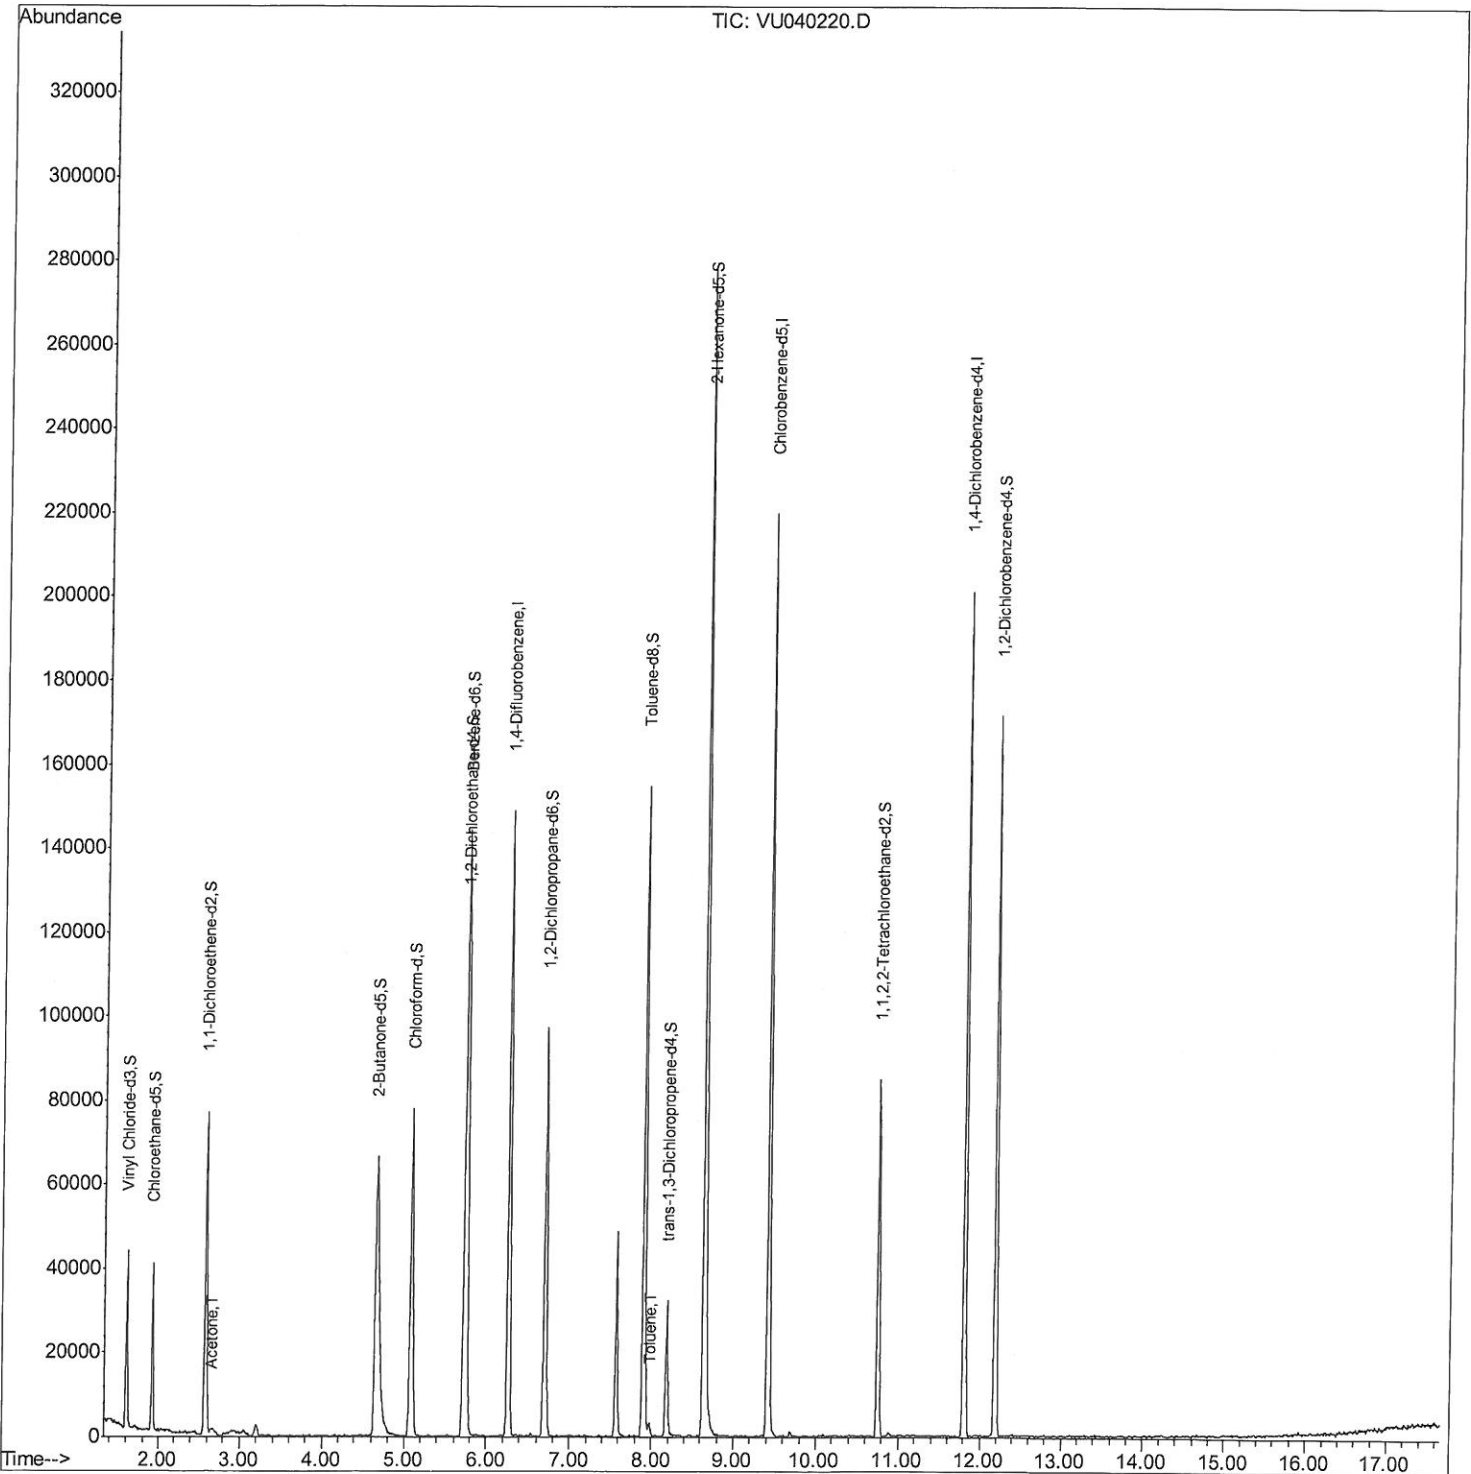

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091820\
 Data File : VU040220.D
 Acq On : 18 Sep 2020 18:45
 Operator : SY/MD
 Sample : L4078-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK9

Manual Integrations
 APPROVED

MMDadoda
 9/21/2020 1:38:14 PM

Quant Time: Sep 18 23:24:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 18 23:20:35 2020
 Response via : Initial Calibration

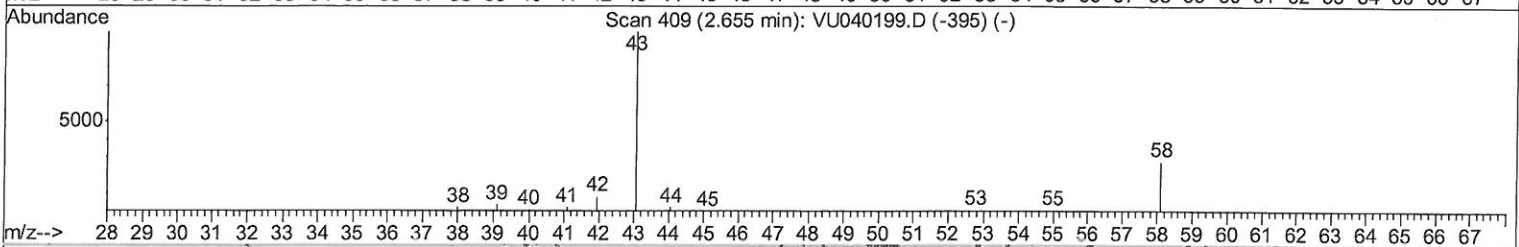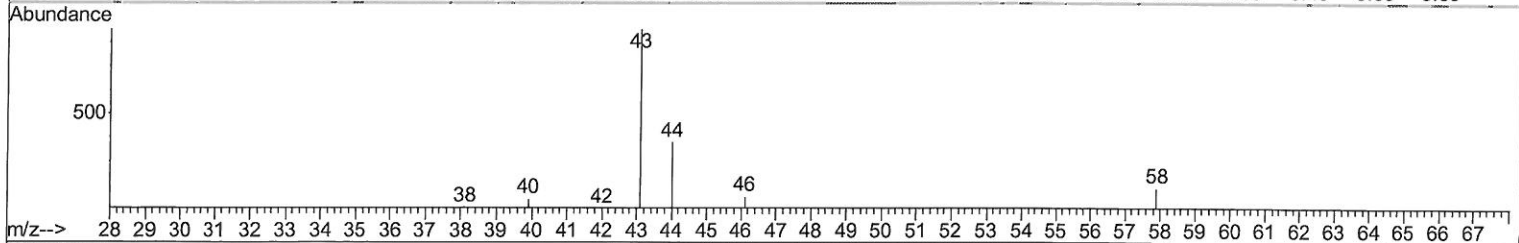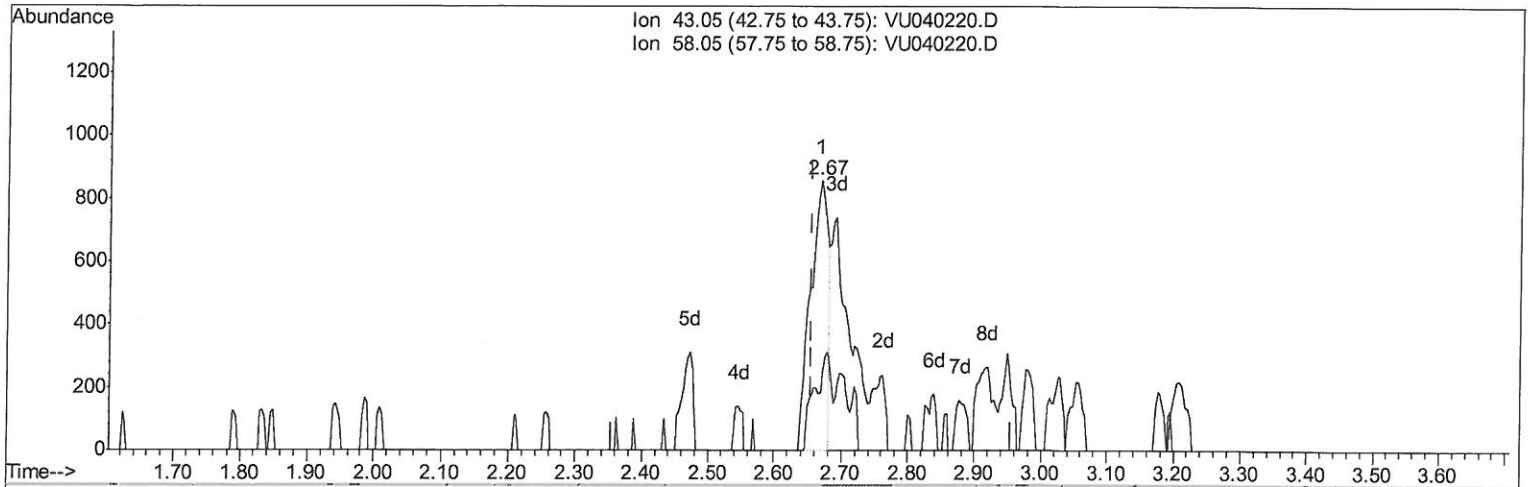

TIC: VU040220.D

(13) Acetone (T)

2.668min (+0.013) 0.70ug/L

response 1563

Ion	Exp%	Act%
43.05	100	100
58.05	27.70	13.12
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091820\
 Data File : VU040220.D
 Acq On : 18 Sep 2020 18:45
 Operator : SY/MD
 Sample : L4078-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 C0AK9

Manual Integrations
APPROVED

MMDadoda
 9/21/2020 1:38:14 PM

Quant Time: Sep 18 23:24:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 18 23:20:35 2020
 Response via : Initial Calibration

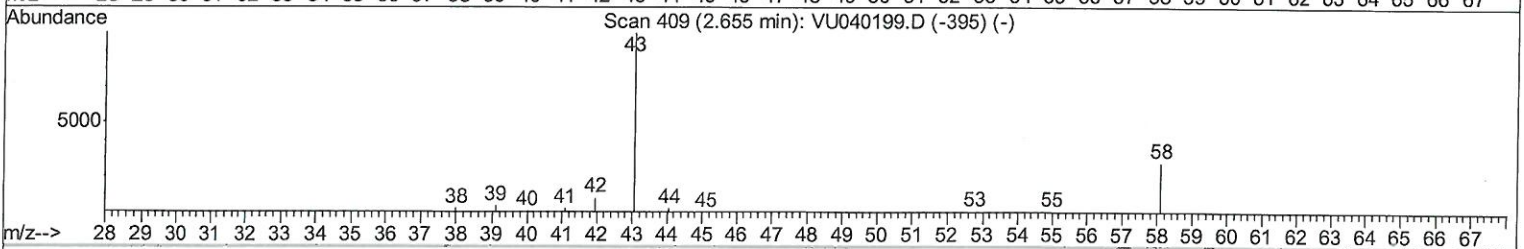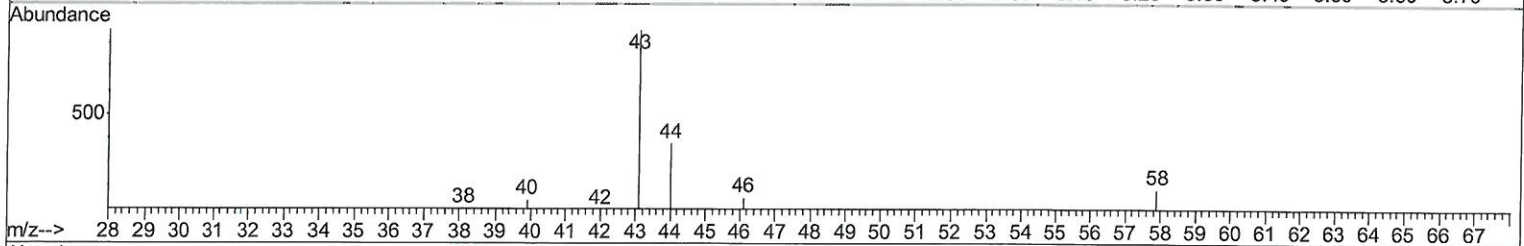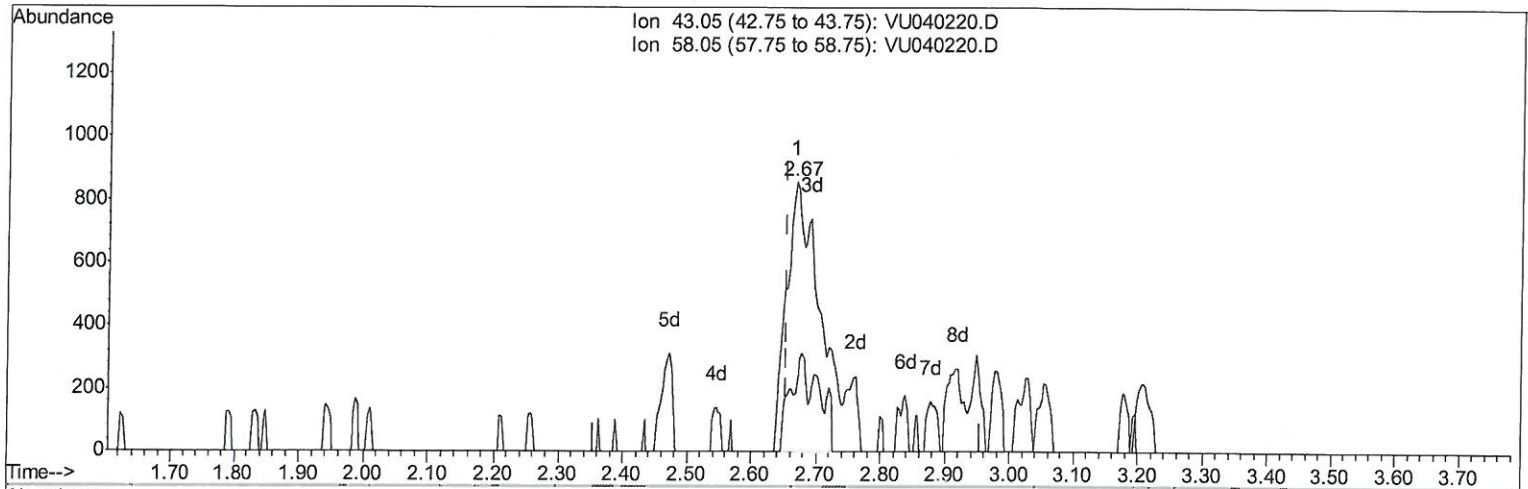

TIC: VU040220.D

(13) Acetone (T)

2.668min (+0.013) 1.48ug/L m

response 3322

Ion	Exp%	Act%
43.05	100	100
58.05	27.70	6.17
0.00	0.00	0.00
0.00	0.00	0.00

7MD
9/21/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091820\
 Data File : VU040220.D
 Acq On : 18 Sep 2020 18:45
 Operator : SY/MD
 Sample : L4078-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK9

Manual Integrations
 APPROVED

MMDadoda
 9/21/2020 1:38:14 PM

Quant Time: Sep 19 01:06:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR083120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Sep 18 23:20:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	110744	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	111998	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	47545	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	26271	4.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.00%
7) Chloroethane-d5	1.92	69	25839	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.60%
11) 1,1-Dichloroethene-d2	2.58	63	48015	3.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.80%
20) 2-Butanone-d5	4.66	46	130329	53.89	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.78%
24) Chloroform-d	5.08	84	67312	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.72	65	44850	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
32) Benzene-d6	5.75	84	119621	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
36) 1,2-Dichloropropane-d6	6.70	67	41978	4.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.40%
41) Toluene-d8	7.90	98	94331	3.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.80%
43) trans-1,3-Dichloropropene-	8.19	79	16383	4.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.80%
46) 2-Hexanone-d5	8.64	63	90668	48.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.70%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	37531	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	39926	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%

Target Compounds

Target Compounds				Ovalue
13) Acetone	2.67	43	3322m	1.484 ug/L
42) Toluene	7.97	91	2381	0.058 ug/L

94 *MD*
 9/21/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed