

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091823\
 Data File : VU055378.D
 Acq On : 18 Sep 2023 18:02
 Operator : MD/SY
 Sample : 04398-03 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4P3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	107	rVB	51378	60096	8.27%	1.228%
2	1.911	184	193	209	rBV	70461	94471	13.01%	1.931%
3	2.563	385	396	412	rBV2	61404	104151	14.34%	2.128%
4	3.042	531	545	558	rBV	17657	32378	4.46%	0.662%
5	3.181	573	588	602	rBV	24365	54575	7.51%	1.115%
6	4.628	1026	1038	1039	rBV2	107399	133944	18.44%	2.737%
7	5.058	1156	1172	1198	rBV2	104903	237335	32.68%	4.850%
8	5.721	1358	1378	1407	rBV4	158496	450569	62.04%	9.208%
9	6.248	1525	1542	1560	rBV	276111	532148	73.27%	10.875%
10	6.541	1620	1633	1652	rBV2	76295	155148	21.36%	3.171%
11	6.689	1663	1679	1699	rBV	155111	308321	42.45%	6.301%
12	7.563	1939	1951	1971	rBV	53415	95321	13.13%	1.948%
13	7.898	2043	2055	2074	rBV	146691	254985	35.11%	5.211%
14	8.180	2131	2143	2158	rBV2	32674	58236	8.02%	1.190%
15	8.634	2272	2284	2327	rBV4	313150	726247	100.00%	14.842%
16	9.415	2514	2527	2548	rBV	328439	553035	76.15%	11.302%
17	10.753	2931	2943	2965	rBV	121895	199016	27.40%	4.067%
18	11.811	3260	3272	3294	rBV	322868	520081	71.61%	10.629%
19	12.190	3379	3390	3411	rBV	193211	323117	44.49%	6.603%




Sum of corrected areas: 4893174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091823\
Data File : VU055378.D
Acq On : 18 Sep 2023 18:02
Operator : MD/SY
Sample : 04398-03 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

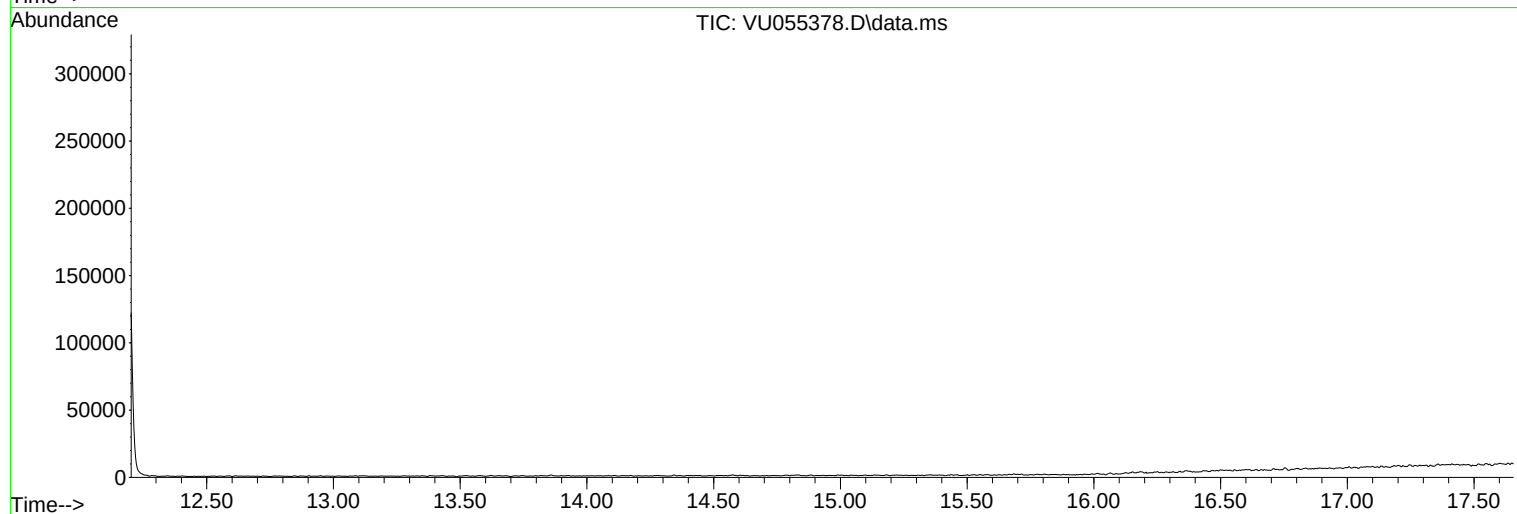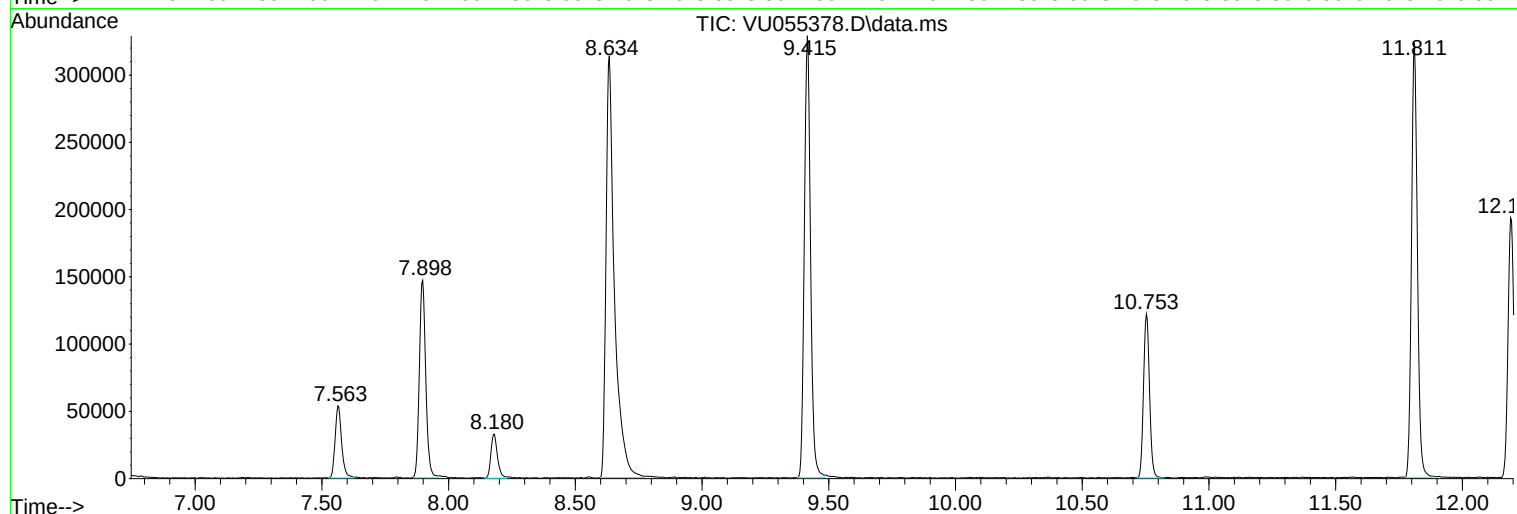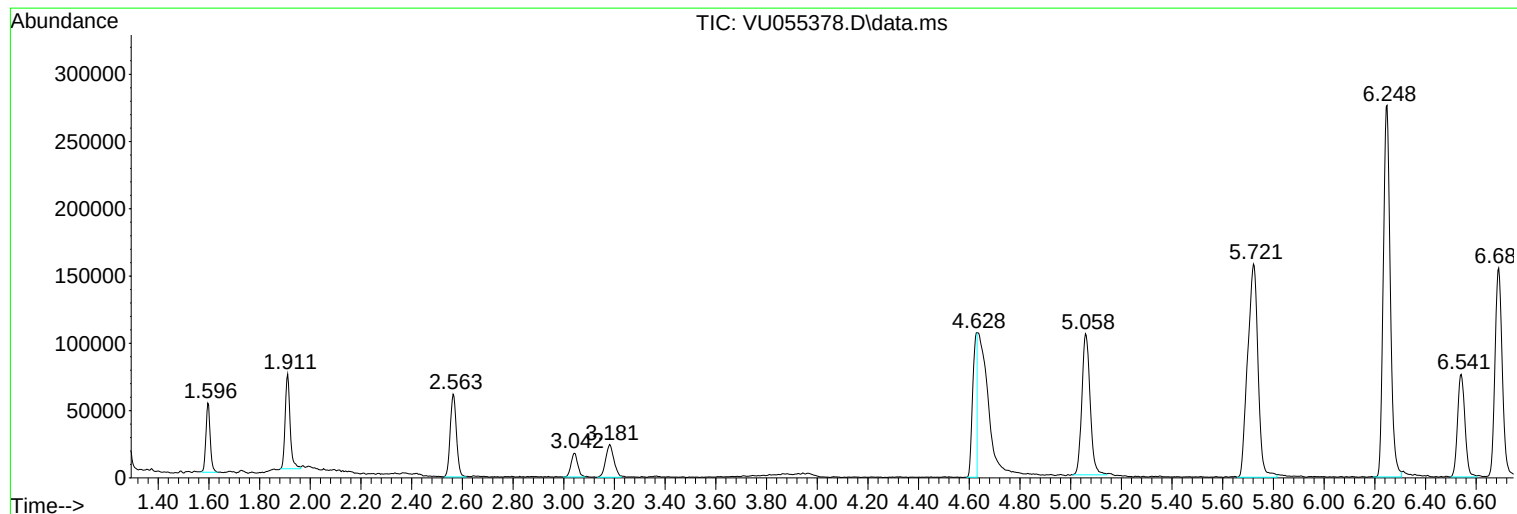

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091823\
Data File : VU055378.D
Acq On : 18 Sep 2023 18:02
Operator : MD/SY
Sample : 04398-03 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091823\
Data File : VU055378.D
Acq On : 18 Sep 2023 18:02
Operator : MD/SY
Sample : 04398-03 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc