


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091823\
Data File : VU055363.D
Acq On : 18 Sep 2023 09:08
Operator : MD/SY
Sample : BFB046
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB046

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091523WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Sep 19 01:12:51 2023

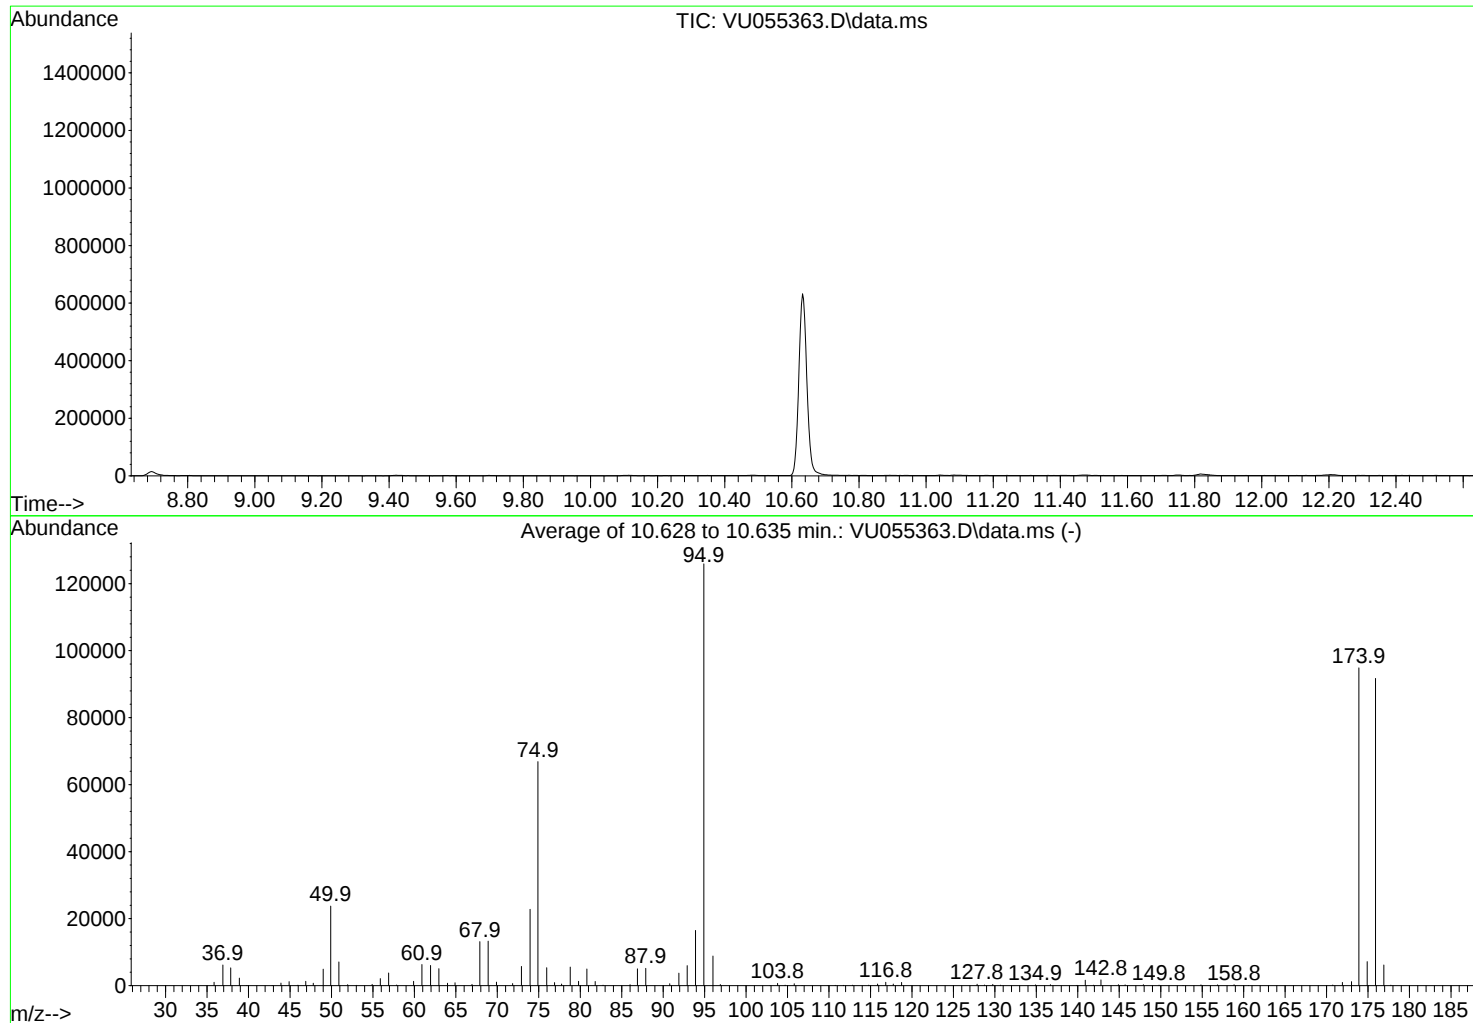

AutoFind: Scans 3078, 3079, 3080; Background Corrected with Scan 3065

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	23731	PASS
75	95	30	80	53.1	66888	PASS
95	95	100	100	100.0	125923	PASS
96	95	5	9	7.0	8848	PASS
173	174	0.00	2	1.2	1182	PASS
174	95	50	120	75.3	94867	PASS
175	174	5	9	7.6	7191	PASS
176	174	95	101	96.7	91699	PASS
177	176	5	9	6.7	6147	PASS

m/z	Abundance
35.80	360.0
37.80	224.0
39.80	146.0
43.90	383.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
35.90	1313.0
36.90	6104.0
37.90	5556.0
38.90	2287.0
39.80	193.0
42.80	110.0
43.90	1208.0
44.90	1033.0
46.00	195.0
46.90	1205.0
47.80	721.0
49.00	4810.0
49.90	23736.0
50.90	7100.0
51.90	209.0
53.00	113.0
54.90	308.0
55.90	1983.0
56.90	3631.0
57.80	224.0
59.90	1270.0
60.90	6417.0
61.90	5958.0
63.00	4888.0
64.00	762.0
64.90	881.0
67.00	383.0
67.90	12997.0
68.90	13091.0
69.90	914.0
71.80	658.0
72.90	5750.0
73.90	22600.0
74.90	65640.0
75.90	5288.0
76.90	913.0
77.80	459.0
78.80	5462.0
79.80	1392.0
80.80	4978.0
81.80	1166.0
82.70	114.0
86.00	335.0
86.90	4882.0
87.90	4943.0
90.80	523.0
91.90	3678.0
92.90	5828.0
93.90	15633.0
94.90	122256.0
96.00	8673.0
96.90	343.0
103.80	725.0
104.70	146.0
105.80	496.0
106.80	124.0
111.70	122.0
112.90	110.0
114.80	138.0
115.80	479.0
116.80	953.0
117.80	409.0
118.70	939.0
127.80	457.0
128.80	109.0
129.80	413.0
130.70	151.0
134.90	248.0
136.70	243.0
139.90	104.0
140.90	1709.0
141.90	102.0
142.80	1612.0
144.90	320.0
145.70	205.0
147.90	269.0
149.80	128.0
154.90	235.0
156.80	211.0
158.80	277.0
170.80	164.0
171.90	752.0
173.00	1127.0
173.90	89888.0
174.90	6652.0
175.90	87080.0
176.90	5664.0
177.80	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
35.90	1390.0
36.90	6283.0
37.90	5683.0
38.90	2283.0
39.90	168.0
42.90	102.0
43.90	1145.0
44.90	1231.0
45.90	153.0
46.90	1302.0
47.80	759.0
49.00	5054.0
49.90	24464.0
50.90	7314.0
52.00	285.0
53.00	112.0
54.90	377.0
55.90	2244.0
56.90	3934.0
57.80	236.0
59.90	1342.0
60.90	6417.0
61.90	6106.0
63.00	5169.0
64.00	742.0
64.90	893.0
66.90	415.0
67.90	13558.0
68.90	13643.0
69.90	1104.0
71.80	632.0
72.90	5927.0
74.00	23312.0
74.90	68992.0
75.90	5369.0
76.90	927.0
77.80	501.0
78.80	5714.0
79.80	1281.0
80.80	5048.0
81.80	1288.0
82.80	121.0
86.00	307.0
86.90	5151.0
87.90	5412.0
90.80	622.0
91.90	3900.0
92.90	6220.0
93.90	17064.0
94.90	129712.0
96.00	9206.0
96.90	320.0
103.80	695.0
104.70	176.0
105.80	595.0
106.70	104.0
109.90	110.0
110.70	115.0
111.80	124.0
112.90	169.0
114.80	149.0
115.80	504.0
116.90	1079.0
117.80	467.0
118.80	1002.0
127.90	440.0
128.80	180.0
129.80	380.0
130.70	147.0
134.90	246.0
136.70	322.0
139.90	126.0
140.90	1734.0
141.90	156.0
142.80	1801.0
144.90	300.0
145.70	269.0
147.90	289.0
149.80	158.0
154.90	269.0
156.80	238.0
158.90	311.0
170.70	203.0
171.90	973.0
173.00	1233.0
173.90	97872.0
174.90	7405.0
175.90	94640.0
176.90	6279.0
177.70	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046

m/z	Abundance
35.90	1455.0
36.90	6137.0
37.90	5362.0
38.90	2115.0
39.90	182.0
43.90	1074.0
44.90	1281.0
45.90	133.0
46.90	1385.0
47.80	692.0
49.00	4948.0
49.90	22992.0
50.90	6766.0
52.00	326.0
53.00	140.0
54.90	394.0
55.90	2139.0
56.90	3774.0
57.90	203.0
59.90	1246.0
60.90	6069.0
62.00	5995.0
62.90	5116.0
64.00	700.0
64.90	846.0
66.90	410.0
67.90	12839.0
68.90	13111.0
69.90	1186.0
71.90	608.0
72.90	5560.0
74.00	22440.0
74.90	66032.0
76.00	5374.0
76.90	826.0
77.70	505.0
78.80	5523.0
79.80	1233.0
80.80	4919.0
81.80	1270.0
82.80	154.0
86.00	201.0
86.90	4967.0
87.90	5175.0
90.80	579.0
91.90	3634.0
92.90	5929.0
93.90	16696.0
94.90	125800.0
96.00	8665.0
96.90	328.0
102.90	124.0
103.80	631.0
104.70	192.0
105.80	623.0
109.90	111.0
110.80	138.0
111.80	104.0
112.80	209.0
114.80	135.0
115.90	484.0
116.90	987.0
117.70	515.0
118.80	897.0
127.90	456.0
128.70	249.0
129.70	325.0
130.70	138.0
134.90	193.0
136.70	293.0
139.90	103.0
140.90	1494.0
141.90	203.0
142.80	1783.0
144.90	268.0
145.70	239.0
147.90	274.0
149.80	196.0
152.70	103.0
154.80	277.0
156.90	284.0
158.90	297.0
160.60	147.0
170.70	195.0
171.90	1170.0
173.00	1185.0
173.90	96840.0
174.90	7515.0
175.90	93376.0
176.90	6499.0
177.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB046