

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091824\
 Data File : VU060865.D
 Acq On : 18 Sep 2024 13:13
 Operator : MD/SY
 Sample : P3973-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ9

Quant Time: Sep 19 05:13:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 19 05:11:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	144998	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	155333	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152	62497	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	41794	3.205	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.000%
7) Chloroethane-d5	1.911	69	35260	3.797	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.000%
11) 1,1-Dichloroethene-d2	2.560	65	16308	3.528	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.600%
20) 2-Butanone-d5	4.638	46	86761	41.440	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.880%
24) Chloroform-d	5.056	84	78016	3.913	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.200%
26) 1,2-Dichloroethane-d4	5.695	65	38624	4.053	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
32) Benzene-d6	5.721	84	151755	3.645	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.000%
36) 1,2-Dichloropropane-d6	6.683	67	51591	4.005	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.200%
41) Toluene-d8	7.891	98	132688	3.496	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.000%
43) trans-1,3-Dichloroprop...	8.178	79	16146	3.482	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.600%
46) 2-Hexanone-d5	8.631	63	68482	37.441	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.880%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	39213	3.886	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	48234	4.593	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.800%
Target Compounds					Qvalue	
13) Acetone	2.657	43	26725	19.133	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091824\
Data File : VU060865.D
Acq On : 18 Sep 2024 13:13
Operator : MD/SY
Sample : P3973-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AQ9


Quant Time: Sep 19 05:13:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 19 05:11:13 2024
Response via : Initial Calibration

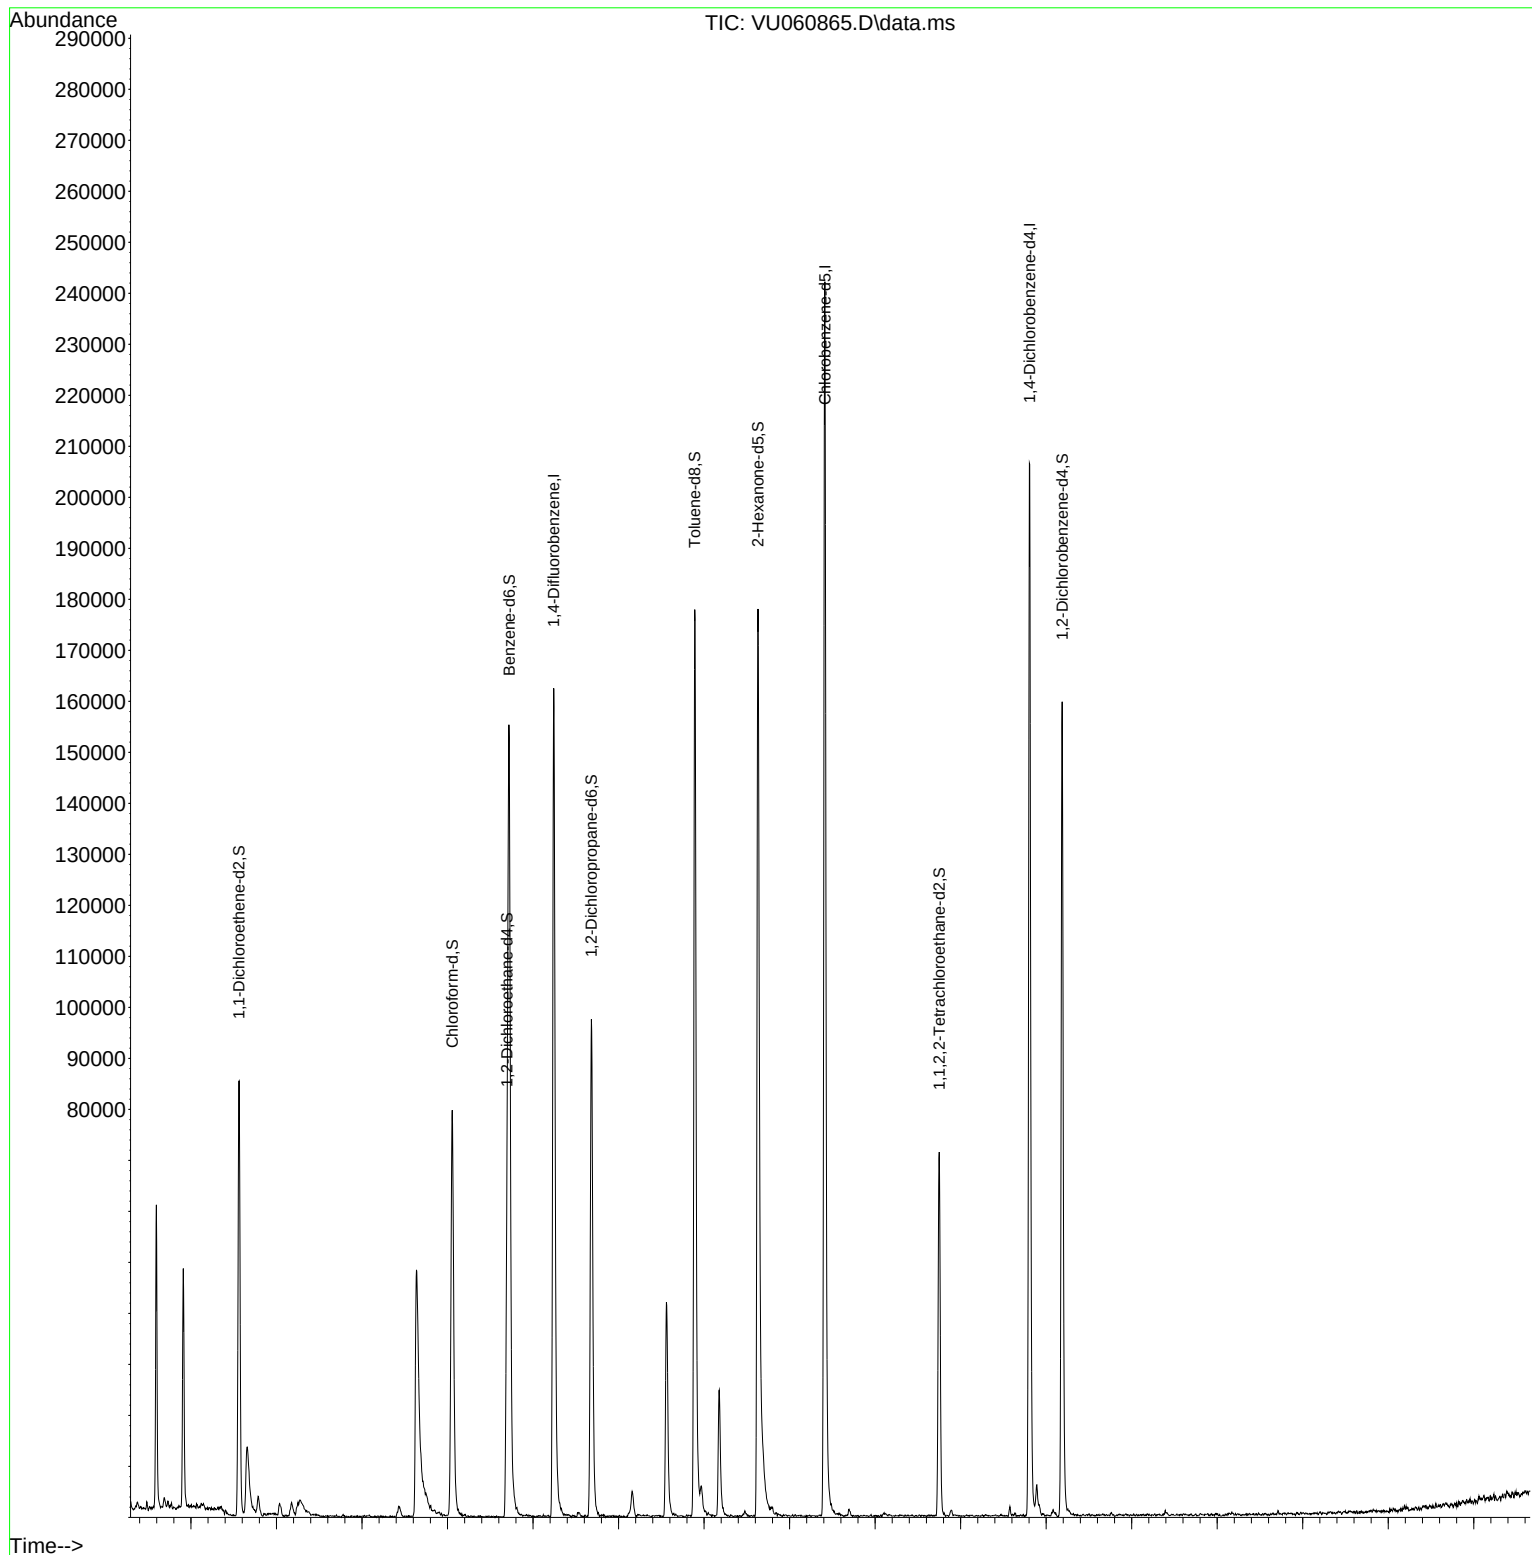

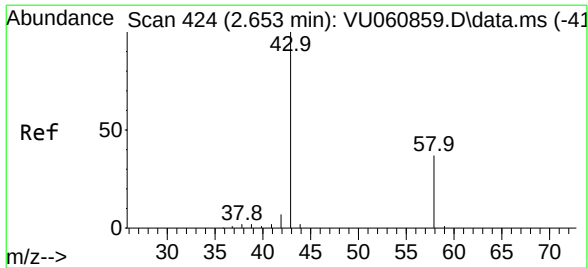

Acetone
 Concen: 19.133 ug/L
 RT: 2.657 min Scan# 42
 Delta R.T. 0.004 min
 Lab File: VU060865.D
 Acq: 18 Sep 2024 13:13

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AQ9

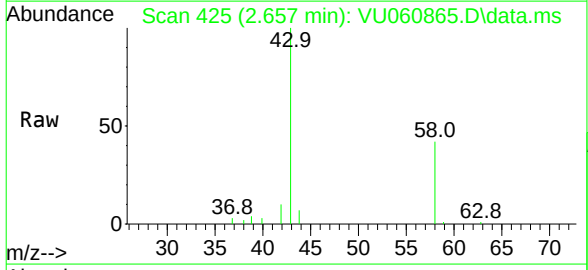

Tgt	Ion: 43	Resp: 26725
Ion	Ratio	Lower Upper
43	100	
58	36.8	0.0 69.6

