

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091918\
 Data File : VU026892.D
 Acq On : 19 Sep 2018 11:38
 Operator : MD/SY
 Sample : VU0919MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	63	69	83	rBV	85615	88744	11.17%	1.468%
2	1.678	149	157	175	rVB	78327	103066	12.98%	1.705%
3	2.270	331	341	354	rBV	151809	231985	29.21%	3.838%
4	2.910	538	540	542	rBV	217	151	0.02%	0.002%
5	2.968	554	558	560	rBV	183	105	0.01%	0.002%
6	3.000	566	568	573	rBV	189	82	0.01%	0.001%
7	3.042	579	581	584	rBV	178	87	0.01%	0.001%
8	3.115	603	604	606	rVB	112	22	0.00%	0.000%
9	3.482	717	718	720	rBV	104	22	0.00%	0.000%
10	3.559	740	742	746	rVB	169	71	0.01%	0.001%
11	3.633	762	765	766	rBV	166	84	0.01%	0.001%
12	3.681	778	780	783	rVB2	182	123	0.02%	0.002%
13	3.730	792	795	798	rBV	176	116	0.01%	0.002%
14	3.794	812	815	822	rBV2	233	229	0.03%	0.004%
15	3.849	831	832	834	rVB2	98	37	0.00%	0.001%
16	4.061	896	898	900	rVB	145	61	0.01%	0.001%
17	4.122	915	917	919	rBV	128	55	0.01%	0.001%
18	4.176	919	934	961	rBV	77953	202437	25.49%	3.349%
19	4.485	1026	1030	1035	rBV	228	181	0.02%	0.003%
20	4.514	1036	1039	1041	rBV	272	111	0.01%	0.002%
21	4.649	1064	1081	1108	rBV	143760	331380	41.73%	5.482%
22	4.881	1147	1153	1164	rVB3	516	1014	0.13%	0.017%
23	4.948	1171	1174	1175	rBV	46	25	0.00%	0.000%
24	4.980	1180	1184	1189	rVV2	308	302	0.04%	0.005%
25	5.029	1197	1199	1203	rBV	156	67	0.01%	0.001%
26	5.051	1203	1206	1209	rVV	170	77	0.01%	0.001%
27	5.064	1209	1210	1212	rVB	123	47	0.01%	0.001%
28	5.090	1215	1218	1222	rBV	71	72	0.01%	0.001%
29	5.196	1249	1251	1253	rBV	90	52	0.01%	0.001%
30	5.241	1262	1265	1267	rBV	87	58	0.01%	0.001%
31	5.340	1272	1296	1320	rBV2	261693	794155	100.00%	13.137%
32	5.537	1353	1357	1359	rBV	65	51	0.01%	0.001%
33	5.553	1359	1362	1365	rVB	46	33	0.00%	0.001%
34	5.646	1388	1391	1394	rBV	67	55	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091918\
 Data File : VU026892.D
 Acq On : 19 Sep 2018 11:38
 Operator : MD/SY
 Sample : VU0919MBL01
 Misc : 5.00µ/5mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

35	5.668	1396	1398	1402	rVB	173	99	0.01%	0.002%
36	5.746	1421	1422	1426	rVB	215	97	0.01%	0.002%
37	5.771	1426	1430	1433	rBV	75	78	0.01%	0.001%
38	5.887	1452	1466	1496	rBV	264592	514388	64.77%	8.509%
39	6.083	1522	1527	1528	rBV	280	147	0.02%	0.002%
40	6.138	1541	1544	1549	rBV2	178	130	0.02%	0.002%
41	6.180	1550	1557	1565	rVB3	561	928	0.12%	0.015%
42	6.221	1565	1570	1573	rBV	64	66	0.01%	0.001%
43	6.257	1577	1581	1584	rBV2	175	114	0.01%	0.002%
44	6.273	1584	1586	1590	rVB	90	52	0.01%	0.001%
45	6.331	1590	1604	1627	rBV	196037	388277	48.89%	6.423%
46	6.440	1636	1638	1639	rBV	126	57	0.01%	0.001%
47	6.504	1653	1658	1660	rBV	121	106	0.01%	0.002%
48	6.537	1665	1668	1670	rBV	87	63	0.01%	0.001%
49	6.598	1683	1687	1689	rBV	124	86	0.01%	0.001%
50	6.617	1692	1693	1698	rVB	211	79	0.01%	0.001%
51	6.646	1698	1702	1705	rBV	96	60	0.01%	0.001%
52	6.665	1705	1708	1710	rBV	77	52	0.01%	0.001%
53	6.720	1724	1725	1727	rBV	87	34	0.00%	0.001%
54	6.733	1727	1729	1734	rBV	70	66	0.01%	0.001%
55	6.762	1735	1738	1739	rBV	103	47	0.01%	0.001%
56	6.800	1747	1750	1751	rBV	121	61	0.01%	0.001%
57	6.855	1761	1767	1769	rBV3	516	501	0.06%	0.008%
58	6.893	1777	1779	1781	rBV	35	16	0.00%	0.000%
59	6.929	1788	1790	1793	rVB	180	83	0.01%	0.001%
60	6.961	1797	1800	1804	rBV	84	67	0.01%	0.001%
61	7.022	1816	1819	1820	rBV	103	64	0.01%	0.001%
62	7.141	1853	1856	1859	rBV	85	72	0.01%	0.001%
63	7.154	1859	1860	1861	rVB	120	24	0.00%	0.000%
64	7.228	1870	1883	1900	rBV	92119	163872	20.63%	2.711%
65	7.366	1924	1926	1927	rBV	253	84	0.01%	0.001%
66	7.408	1938	1939	1940	rBV	110	26	0.00%	0.000%
67	7.472	1957	1959	1964	rVB	185	97	0.01%	0.002%
68	7.511	1970	1971	1972	rBV	135	41	0.01%	0.001%
69	7.569	1976	1989	2017	rBV	314622	547090	68.89%	9.050%
70	7.755	2045	2047	2050	rVB	201	94	0.01%	0.002%
71	7.781	2050	2055	2058	rVB2	316	223	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU091918\
 Data File : VU026892.D
 Acq On : 19 Sep 2018 11:38
 Operator : MD/SY
 Sample : VU0919MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
 Title : VOC Analysis

72	7.852	2064	2077	2098	rBV	66845	114772	14.45%	1.899%
73	7.980	2114	2117	2121	rVB2	283	254	0.03%	0.004%
74	8.003	2121	2124	2126	rBV	217	147	0.02%	0.002%
75	8.077	2145	2147	2148	rBV	126	39	0.00%	0.001%
76	8.102	2153	2155	2157	rVB	135	45	0.01%	0.001%
77	8.173	2170	2177	2179	rBV	662	673	0.08%	0.011%
78	8.311	2208	2220	2256	rBV	240679	419324	52.80%	6.937%
79	8.617	2305	2315	2324	rVB4	1825	2879	0.36%	0.048%
80	8.659	2324	2328	2329	rBV	169	103	0.01%	0.002%
81	8.697	2338	2340	2345	rVB	153	78	0.01%	0.001%
82	8.758	2356	2359	2362	rBV2	211	154	0.02%	0.003%
83	8.835	2381	2383	2385	rBV	144	83	0.01%	0.001%
84	9.009	2436	2437	2439	rVB	143	31	0.00%	0.001%
85	9.025	2439	2442	2445	rBV	199	123	0.02%	0.002%
86	9.093	2447	2463	2489	rBV	382598	631376	79.50%	10.444%
87	9.241	2504	2509	2513	rBV2	369	380	0.05%	0.006%
88	9.308	2527	2530	2534	rBV	192	196	0.02%	0.003%
89	9.369	2546	2549	2550	rBV	186	82	0.01%	0.001%
90	9.427	2565	2567	2569	rBV	176	96	0.01%	0.002%
91	9.562	2606	2609	2610	rBV	153	88	0.01%	0.001%
92	9.601	2618	2621	2622	rBV	160	73	0.01%	0.001%
93	9.996	2742	2744	2746	rBV	153	69	0.01%	0.001%
94	10.433	2866	2880	2900	rBV	289111	454021	57.17%	7.511%
95	10.536	2911	2912	2921	rBV	222	140	0.02%	0.002%
96	11.485	3195	3207	3226	rBV	324774	502798	63.31%	8.317%
97	11.861	3312	3324	3345	rBV	339324	544519	68.57%	9.008%


Sum of corrected areas: 6045141

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU091918\
Data File : VU026892.D
Acq On : 19 Sep 2018 11:38
Operator : MD/SY
Sample : VU0919MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VBLK46

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

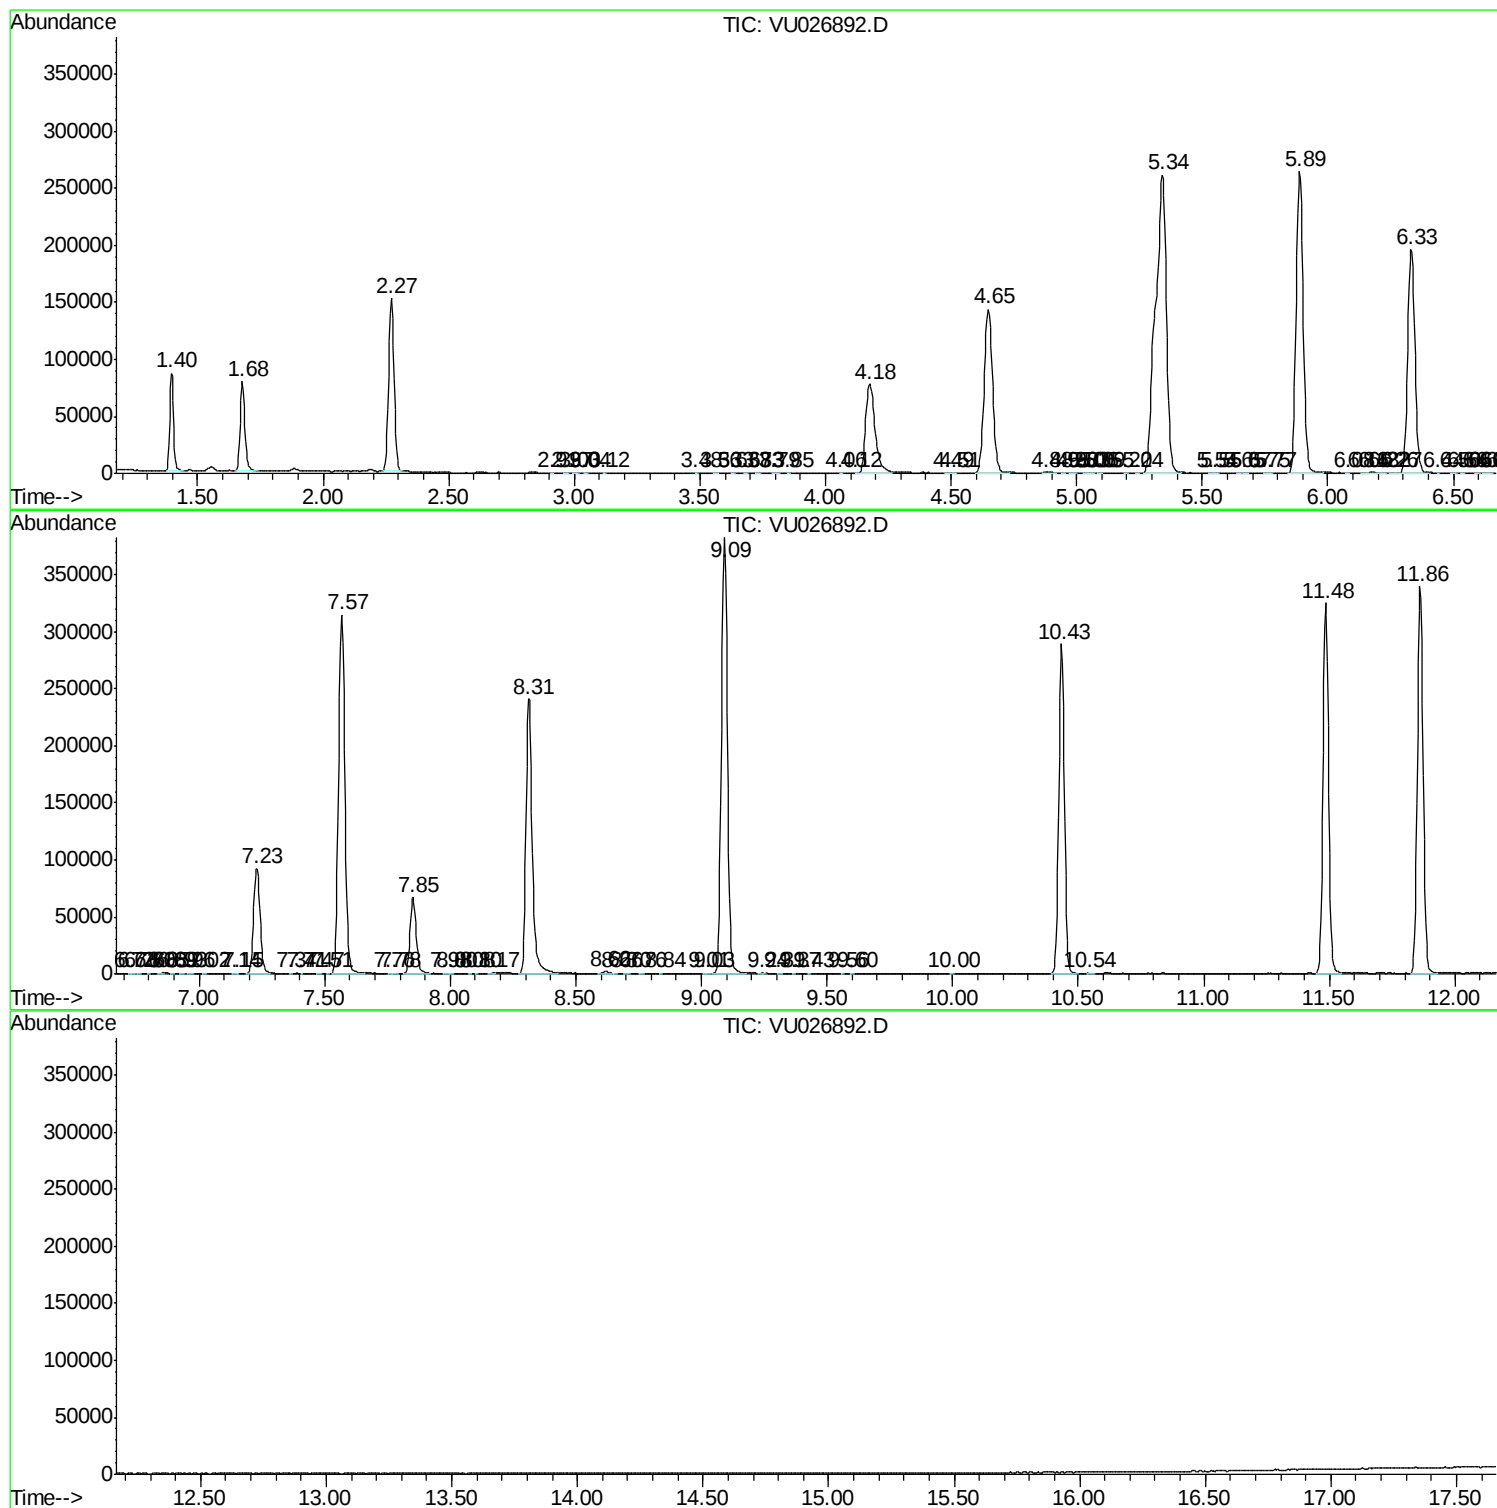

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091918\
Data File : VU026892.D
Acq On : 19 Sep 2018 11:38
Operator : MD/SY
Sample : VU0919MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK46

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU091918\
Data File : VU026892.D
Acq On : 19 Sep 2018 11:38
Operator : MD/SY
Sample : VU0919MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK46

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc