


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091918\
Data File : VU026889.D
Acq On : 19 Sep 2018 10:06
Operator : MD/SY
Sample : BFB42
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091718WMA.M
Title : VOC Analysis
Last Update : Fri Sep 21 04:24:07 2018

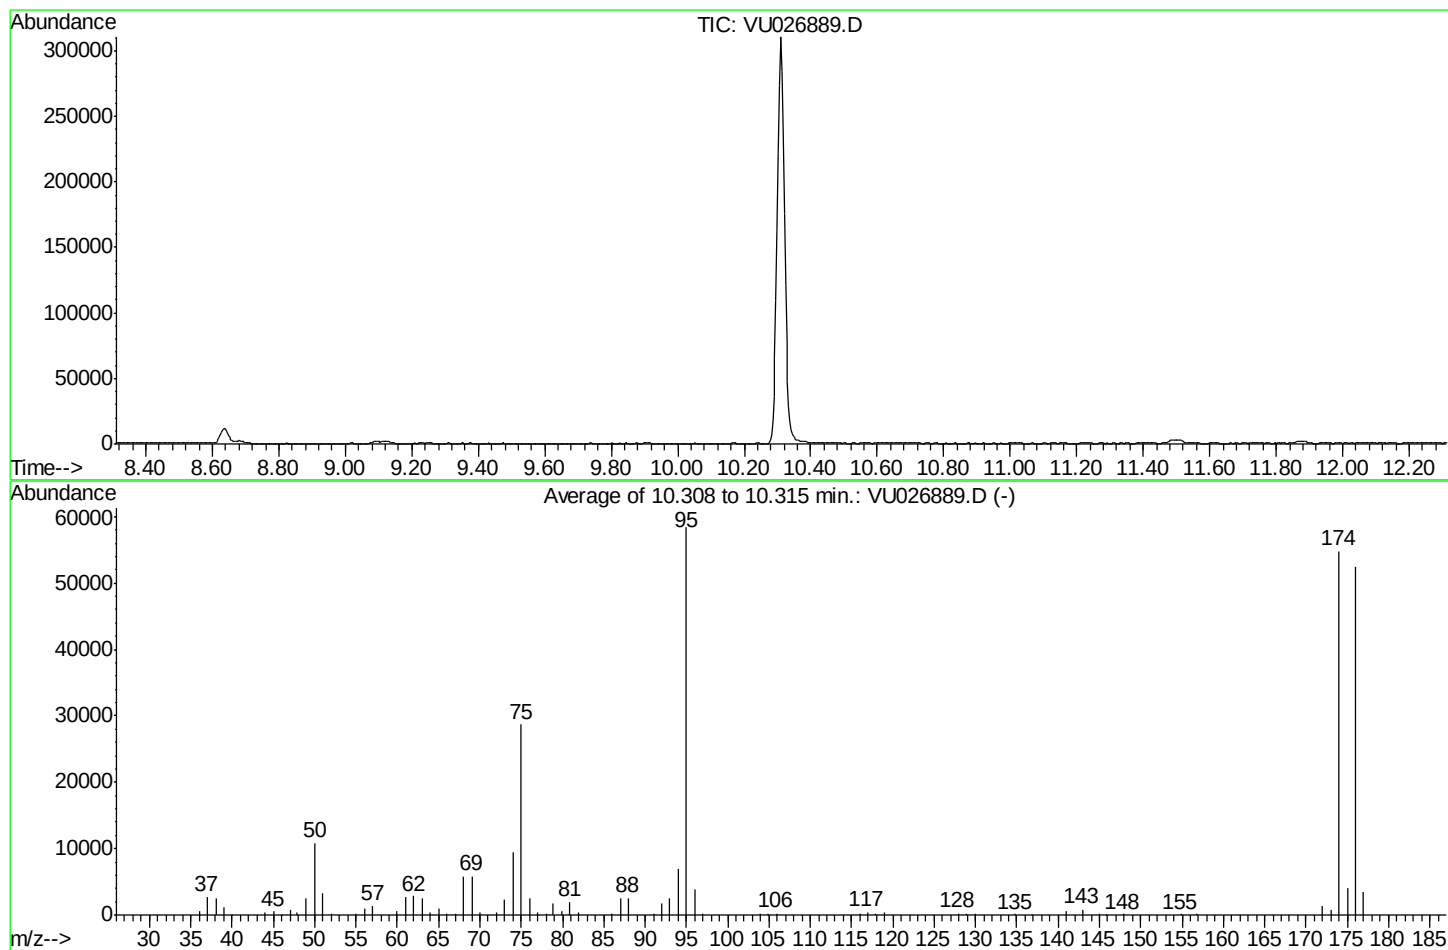

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	10816	PASS
75	95	30	80	49.1	28701	PASS
95	95	100	100	100.0	58400	PASS
96	95	5	9	6.8	3947	PASS
173	174	0.00	2	1.4	764	PASS
174	95	50	120	93.9	54853	PASS
175	174	5	9	7.5	4134	PASS
176	174	95	101	95.6	52453	PASS
177	176	5	9	6.6	3455	PASS

m/z	Abundance
44.00	421.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	579.0
37.00	2932.0
38.00	2583.0
39.00	1195.0
44.00	756.0
45.00	545.0
46.00	113.0
47.00	815.0
47.90	344.0
49.00	2720.0
50.00	11123.0
51.00	3544.0
52.00	137.0
55.00	189.0
56.10	951.0
57.00	1460.0
60.00	569.0
61.00	2927.0
62.00	2935.0
63.00	2675.0
64.00	496.0
65.00	964.0
66.00	125.0
67.00	204.0
68.00	5796.0
69.00	6045.0
70.00	493.0
72.10	341.0
73.00	2499.0
74.00	9803.0
75.00	29744.0
76.00	2593.0
76.90	332.0
78.00	293.0
78.90	1864.0
80.00	545.0
80.90	1949.0
81.90	420.0
86.00	121.0
87.00	2552.0
88.00	2679.0
91.00	238.0
92.00	1718.0
93.00	2562.0
94.00	7100.0
95.00	59592.0
96.00	4052.0
97.00	171.0
103.90	232.0
104.90	100.0
105.90	253.0
115.90	175.0
116.90	481.0
117.90	262.0
118.90	342.0
127.90	231.0
128.80	103.0
129.90	204.0
134.90	133.0
136.80	148.0
140.90	563.0
142.90	874.0
144.90	260.0
145.80	101.0
147.90	159.0
154.90	144.0
156.80	128.0
172.00	1388.0
173.00	733.0
174.00	55112.0
175.00	4168.0
176.00	52232.0
177.00	3560.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	573.0
37.00	2828.0
38.00	2609.0
39.00	1210.0
44.00	771.0
45.00	560.0
46.00	114.0
47.00	755.0
47.90	335.0
49.00	2561.0
50.10	11196.0
51.00	3462.0
52.00	133.0
55.00	182.0
56.10	950.0
57.00	1408.0
60.00	602.0
61.00	2775.0
62.00	2904.0
63.00	2588.0
64.00	432.0
65.00	923.0
66.00	122.0
67.00	196.0
68.00	5943.0
69.00	5987.0
70.00	495.0
72.00	311.0
73.00	2417.0
74.00	9861.0
75.00	29720.0
76.00	2601.0
77.00	333.0
78.00	294.0
78.90	1854.0
79.90	525.0
80.90	1989.0
81.90	439.0
85.90	116.0
87.00	2532.0
88.00	2652.0
91.00	240.0
92.00	1722.0
93.00	2511.0
94.00	7280.0
95.00	60224.0
96.00	4143.0
97.00	157.0
104.00	217.0
104.90	112.0
105.90	306.0
116.00	203.0
116.90	513.0
117.90	307.0
118.90	395.0
127.90	212.0
128.80	124.0
129.90	203.0
134.80	134.0
136.80	126.0
140.90	518.0
142.90	790.0
145.00	258.0
148.00	164.0
154.80	153.0
156.80	132.0
172.00	1437.0
173.00	795.0
174.00	56728.0
175.00	4285.0
176.00	54384.0
177.00	3570.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	491.0
37.00	2454.0
38.10	2382.0
39.00	1119.0
40.00	113.0
44.00	751.0
45.00	496.0
47.00	628.0
47.90	298.0
49.00	2130.0
50.10	10131.0
51.00	3030.0
52.00	141.0
55.00	160.0
56.00	833.0
57.00	1235.0
60.00	553.0
61.00	2395.0
62.00	2610.0
63.00	2251.0
64.00	344.0
65.00	813.0
66.10	114.0
67.00	147.0
68.00	5516.0
69.00	5367.0
70.00	479.0
72.00	261.0
73.00	2172.0
74.00	8951.0
75.00	26640.0
76.00	2344.0
77.00	299.0
78.00	226.0
78.90	1738.0
79.90	458.0
80.90	1874.0
81.90	399.0
85.80	111.0
87.00	2304.0
87.90	2288.0
91.00	234.0
92.00	1598.0
93.00	2232.0
94.00	6719.0
95.00	55384.0
96.00	3646.0
96.90	122.0
104.00	178.0
104.90	104.0
105.90	283.0
116.00	182.0
116.90	461.0
117.90	266.0
118.90	388.0
127.90	178.0
128.90	120.0
129.90	187.0
134.80	109.0
140.90	483.0
143.00	661.0
145.00	223.0
148.00	138.0
154.80	137.0
156.80	122.0
172.00	1288.0
173.00	766.0
174.00	52720.0
175.00	3949.0
176.00	50744.0
177.00	3235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42