


Data File : VU034673.D
Acq On : 20 Sep 2019 01:43
Operator : JC/SP
Sample : K4895-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 20 07:20:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 20 04:02:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampled :
BFDG1

Manual Integrations
APPROVED

MMDadoda
9/20/2019 12:46:35 PM

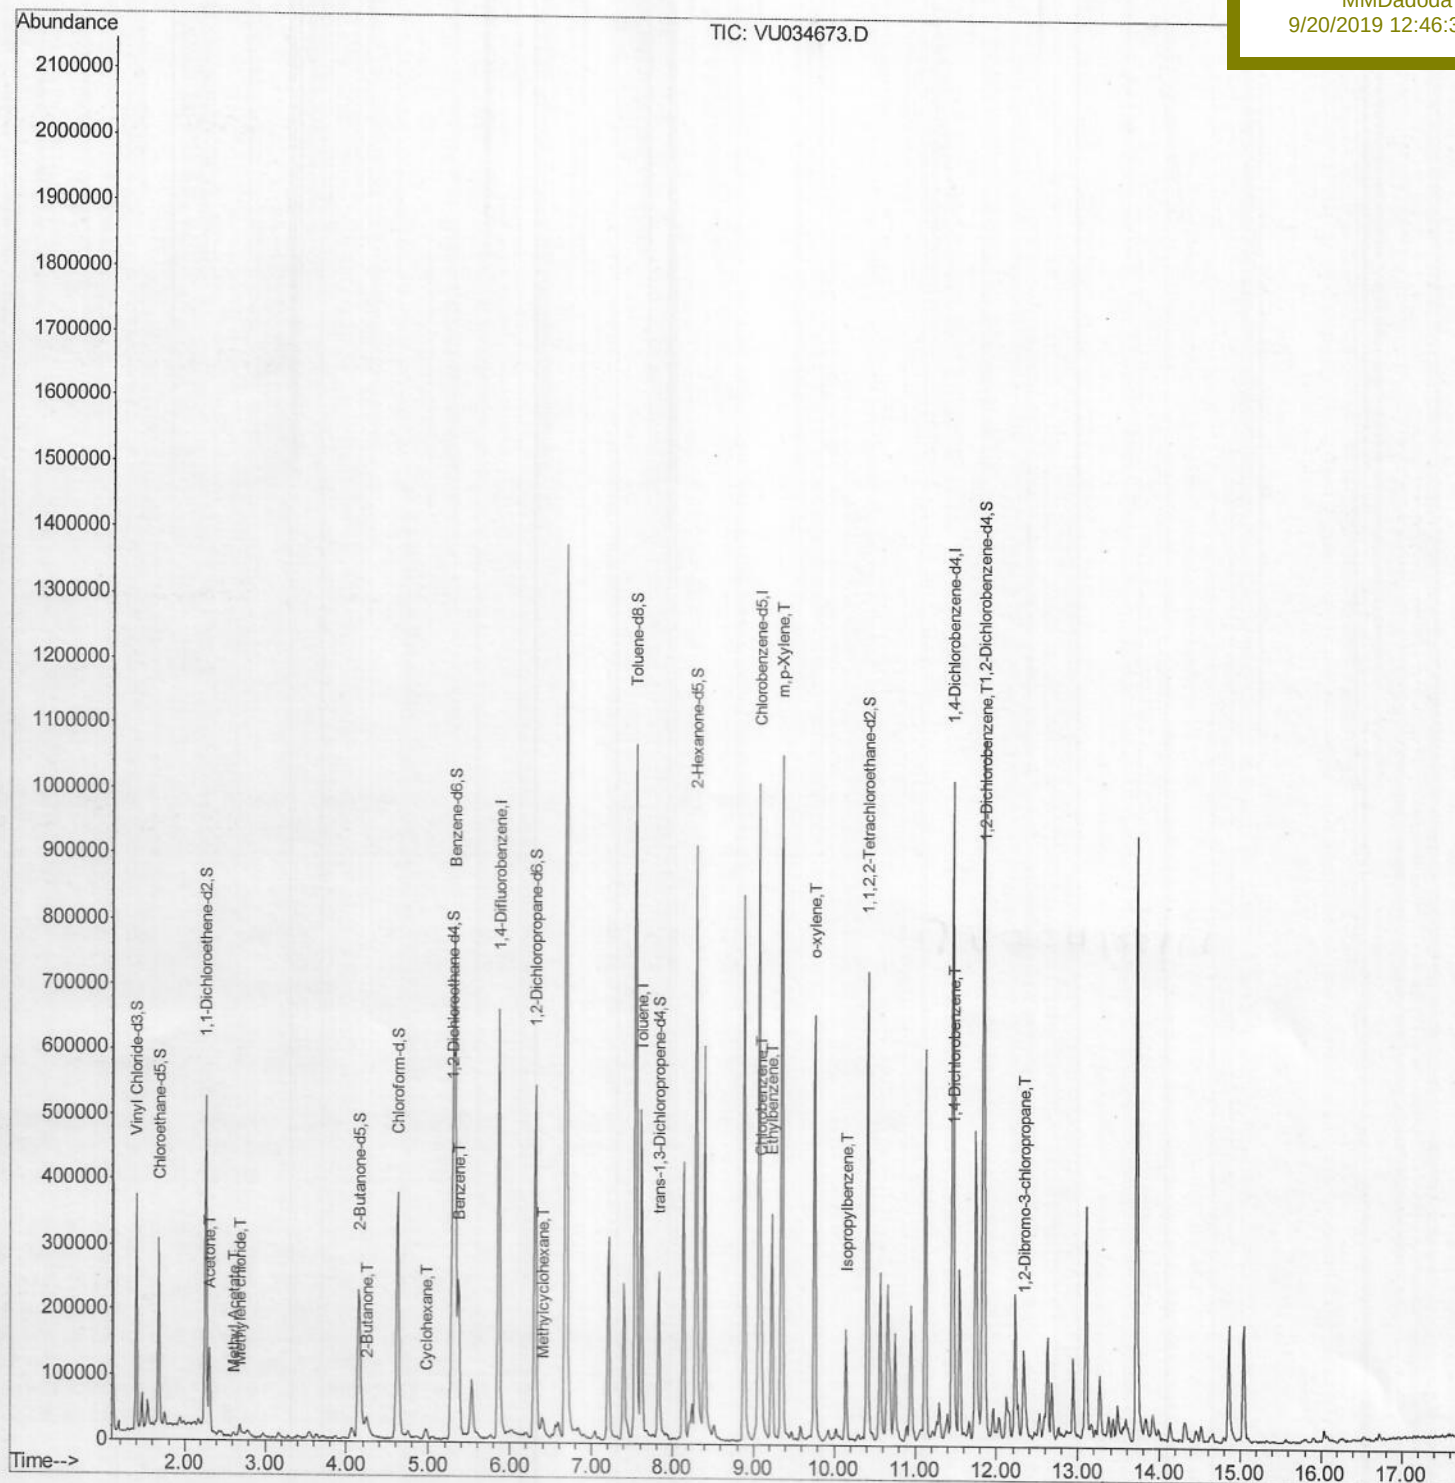




Data File : VU034673.D
Acq On : 20 Sep 2019 01:43
Operator : JC/SP
Sample : K4895-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 20 04:10:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 20 04:02:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
BFDG1

Manual Integrations
APPROVED

MMDadoda
9/20/2019 12:46:35 PM

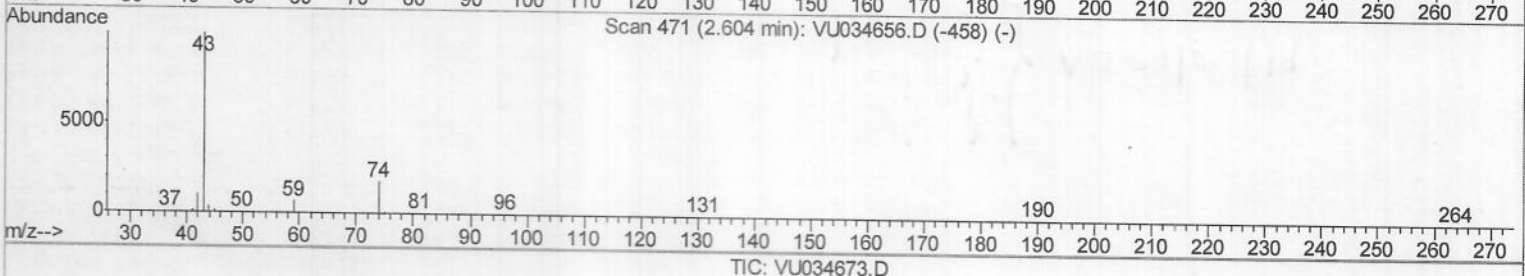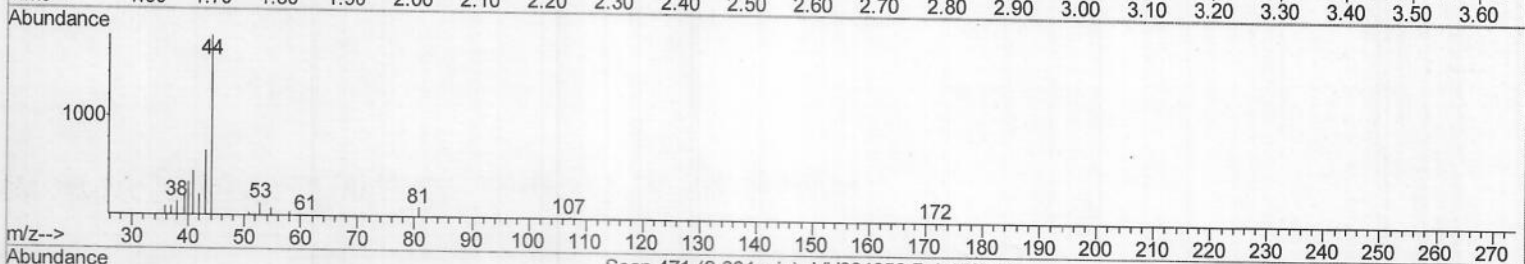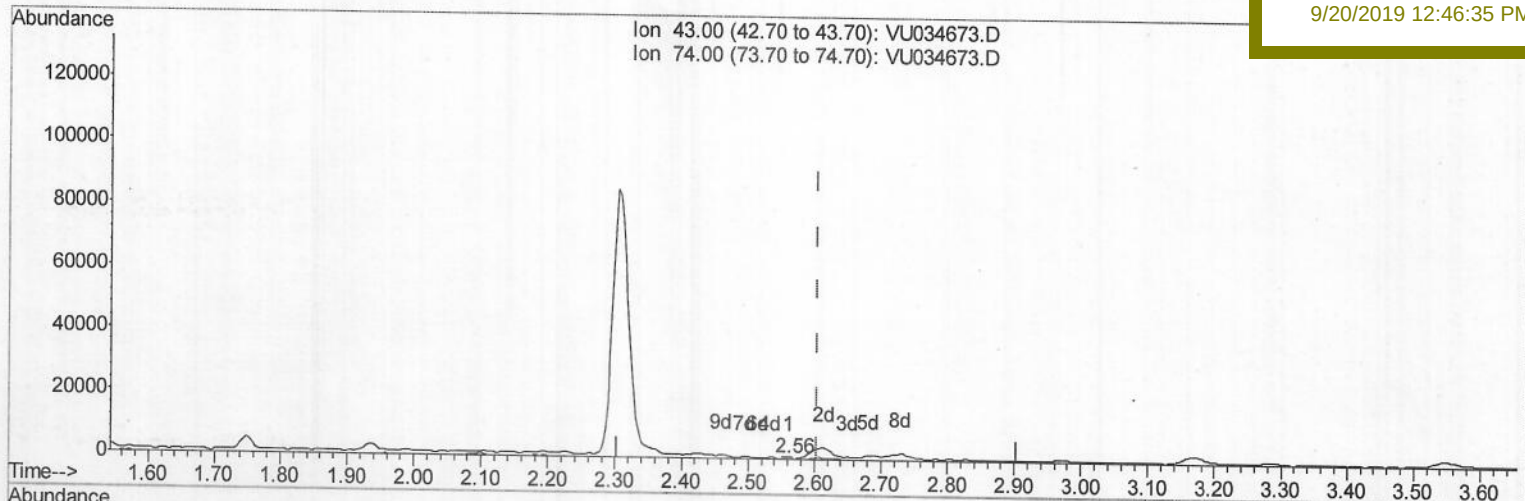

TIC: VU034673.D

(15) Methyl Acetate (T)

2.563min (-0.042) 0.05ug/L

response 317

Ion	Exp%	Act%
43.00	100	100
74.00	18.00	17.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU091919\
Quantitation Report (Qedit)




Data File : VU034673.D
Acq On : 20 Sep 2019 01:43
Operator : JC/SP
Sample : K4895-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 20 04:10:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 20 04:02:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
BFDG1

Manual Integrations
APPROVED

MMDadoda
9/20/2019 12:46:35 PM

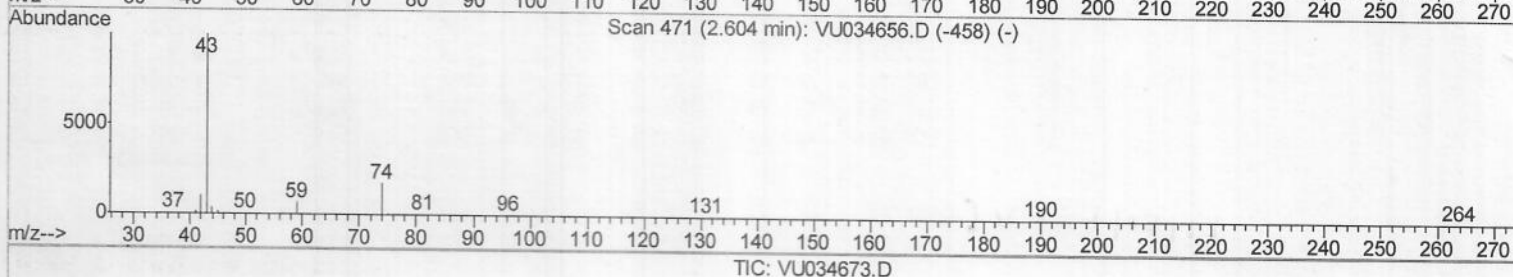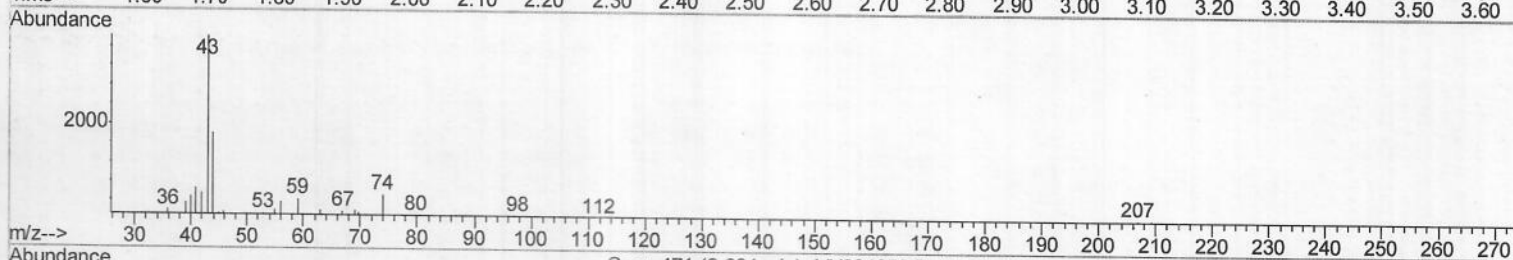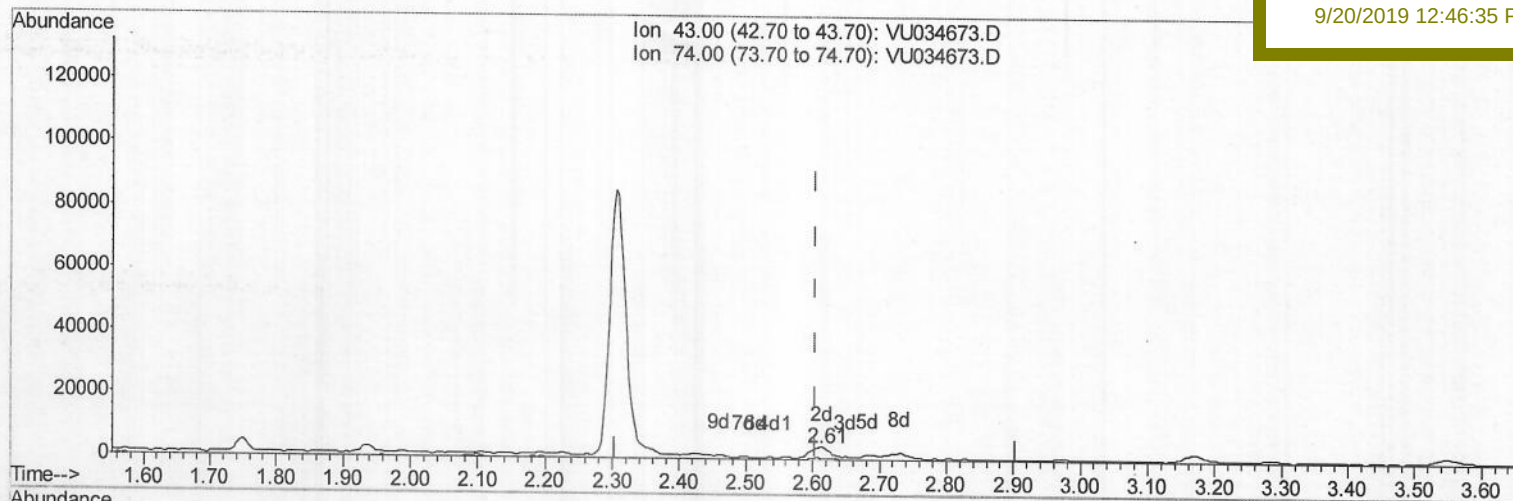

TIC: VU034673.D

(15) Methyl Acetate (T)

2.614min (+0.010) 1.36ug/L m

response 8286

Ion Exp% Act%

43.00 100 100

74.00 18.00 0.68#

0.00 0.00 0.00

0.00 0.00 0.00

M.A
09/20/19

Data File : VU034673.D

Acq On : 20 Sep 2019 01:43

Operator : JC/SP

Sample : K4895-15

Misc : 5.0mL/MSVOA_U/WATER

ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 20 07:20:44 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M

Quant Title : VOC Analysis

QLast Update : Fri Sep 20 04:02:05 2019

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :

BFDG1

Manual Integrations

APPROVED

MMDadoda

9/20/2019 12:46:35 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	499110	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	477468	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	228039	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	221078	43.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.54%
7) Chloroethane-d5	1.67	69	182483	46.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.42%
11) 1,1-Dichloroethene-d2	2.26	63	300667	34.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.50%
21) 2-Butanone-d5	4.15	46	402436	102.77	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.77%
24) Chloroform-d	4.62	84	353048	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.06%
26) 1,2-Dichloroethane-d4	5.29	65	256041	46.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.78%
32) Benzene-d6	5.32	84	705597	47.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.36%
36) 1,2-Dichloropropane-d6	6.31	67	247821	47.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.82%
41) Toluene-d8	7.54	98	667596	47.41	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.82%
43) trans-1,3-Dichloropropene-	7.83	79	113486	45.81	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.62%
47) 2-Hexanone-d5	8.29	63	268204	103.23	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.23%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	337083	46.96	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.92%
64) 1,2-Dichlorobenzene-d4	11.84	152	231603	48.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.86%

Target Compounds

					Qvalue
13) Acetone	2.31	43	141267	31.011 ug/L	99
15) Methyl Acetate	2.61	43	8286m	1.362 ug/L	
16) Methylene chloride	2.68	84	5536	1.338 ug/L	96
22) 2-Butanone	4.25	43	48094	8.874 ug/L	96
29) Cyclohexane	4.97	56	6591	0.836 ug/L #	41
33) Benzene	5.37	78	199666	12.057 ug/L	100
35) Methylcyclohexane	6.39	83	7932	1.143 ug/L	90
42) Toluene	7.62	91	345105	19.283 ug/L	98
51) Chlorobenzene	9.10	112	89631	8.239 ug/L	97
52) Ethylbenzene	9.23	91	235943	11.708 ug/L	100
53) m,p-Xylene	9.35	106	270198	37.853 ug/L	97
54) o-xylene	9.76	106	143139	20.274 ug/L	98
56) Isopropylbenzene	10.14	105	100995	5.305 ug/L	98
63) 1,4-Dichlorobenzene	11.48	146	19711	2.450 ug/L	91
65) 1,2-Dichlorobenzene	11.85	146	41629	5.217 ug/L	98
66) 1,2-Dibromo-3-chloropropan	12.33	75	2181	1.286 ug/L #	10

M.A
09/20/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU091919\
Quantitation Report (QT Reviewed)

Data File : VU034673.D
Acq On : 20 Sep 2019 01:43
Operator : JC/SP
Sample : K4895-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 20 07:20:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 20 04:02:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
BFDG1

Manual Integrations
APPROVED

MMDadoda
9/20/2019 12:46:35 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed