


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091919\
 Data File : VU034648.D
 Acq On : 19 Sep 2019 14:34
 Operator : JC/SP
 Sample : BFB34
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB34

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 28 02:29:26 2019

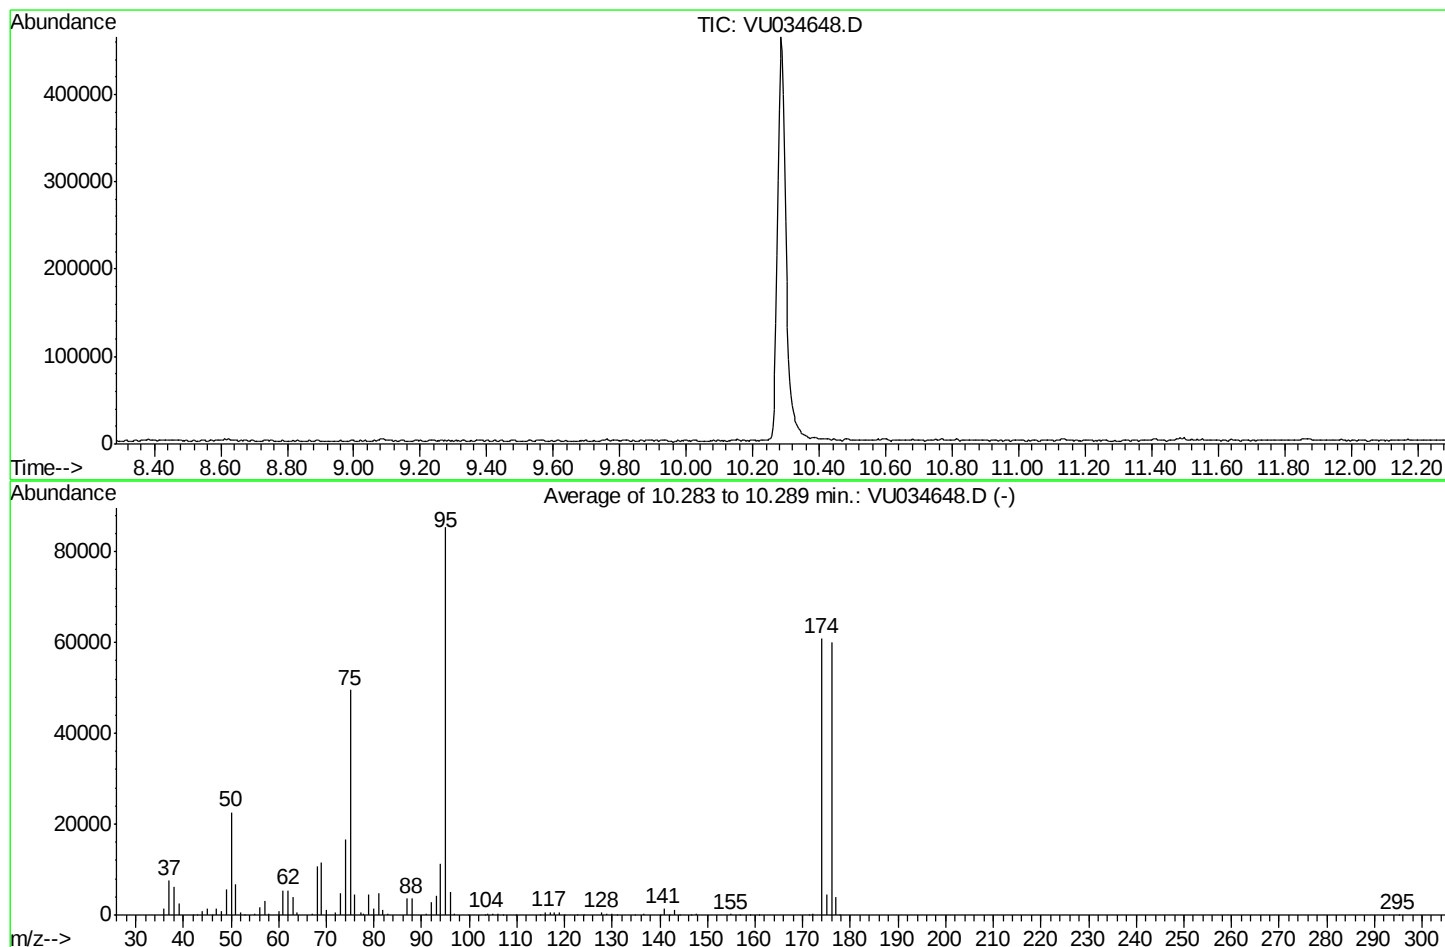

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.5	22624	PASS
75	95	30	80	58.0	49538	PASS
95	95	100	100	100.0	85354	PASS
96	95	5	9	5.9	5055	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.3	60834	PASS
175	174	5	9	7.2	4405	PASS
176	174	95	101	98.8	60082	PASS
177	176	5	9	6.7	4028	PASS

m/z	Abundance
37.90	191.0
39.10	220.0
39.90	521.0
41.00	185.0
41.80	112.0
43.00	119.0
44.00	1221.0
45.00	156.0
54.90	185.0
56.00	137.0
56.90	190.0
67.40	103.0
68.00	223.0
73.00	128.0
96.00	193.0
106.10	132.0
141.50	117.0
207.00	251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
35.90	1492.0
37.00	7393.0
38.00	6299.0
39.00	2818.0
40.00	395.0
41.00	138.0
42.10	131.0
42.90	157.0
44.00	2067.0
45.00	1586.0
46.10	203.0
47.00	1375.0
47.90	947.0
49.00	5469.0
50.00	22536.0
51.00	7187.0
51.90	393.0
52.90	153.0
55.00	305.0
56.00	1878.0
57.10	3274.0
58.00	180.0
60.00	842.0
61.00	5369.0
62.00	5231.0
63.00	4025.0
64.00	495.0
67.10	285.0
68.00	11335.0
69.00	11349.0
70.00	1274.0
71.90	688.0
73.00	5003.0
74.00	16640.0
75.00	48096.0
76.00	4598.0
77.20	552.0
77.90	383.0
78.90	4496.0
79.90	1404.0
80.90	4648.0
81.90	1261.0
82.90	209.0
87.00	3766.0
88.00	3630.0
90.90	389.0
92.00	2717.0
93.00	3946.0
94.00	10960.0
95.00	81728.0
96.00	5139.0
96.90	198.0
103.20	131.0
103.90	446.0
104.80	368.0
105.90	470.0
109.80	182.0
115.00	158.0
115.90	374.0
117.00	666.0
117.90	565.0
119.00	682.0
119.90	106.0
123.90	168.0
127.90	355.0
128.90	133.0
130.00	346.0
134.80	113.0
136.70	127.0
140.20	107.0
140.90	1350.0
142.90	1179.0
144.20	152.0
146.60	211.0
147.70	222.0
155.00	155.0
158.80	119.0
172.00	112.0
174.00	58760.0
175.00	4385.0
176.00	57152.0
176.90	3973.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	1521.0
37.00	7719.0
38.00	6524.0
39.00	2744.0
39.90	439.0
41.00	105.0
43.00	209.0
44.00	2148.0
45.00	1604.0
46.00	163.0
46.90	1551.0
47.90	904.0
49.00	5929.0
50.00	23392.0
51.00	6959.0
51.90	501.0
52.80	160.0
54.90	431.0
56.00	2034.0
57.00	3410.0
57.90	253.0
59.90	910.0
61.00	5402.0
62.00	5494.0
63.00	4059.0
64.00	487.0
67.00	290.0
68.00	11324.0
69.00	12094.0
70.00	1200.0
71.90	597.0
73.00	5030.0
74.00	17008.0
75.00	51192.0
76.00	4491.0
77.10	691.0
77.80	326.0
78.90	4614.0
79.90	1384.0
81.00	4799.0
81.90	1246.0
82.80	153.0
86.90	3688.0
87.90	3682.0
91.00	424.0
92.00	2963.0
93.00	4523.0
94.00	11468.0
95.00	88048.0
96.00	5488.0
96.90	267.0
100.00	104.0
103.20	127.0
103.80	398.0
104.90	316.0
106.00	513.0
109.80	146.0
115.00	121.0
115.90	454.0
117.00	771.0
117.90	482.0
119.00	634.0
119.90	123.0
122.70	102.0
123.90	134.0
127.80	448.0
128.80	156.0
130.00	426.0
134.70	114.0
136.80	221.0
140.10	138.0
140.90	1382.0
141.90	124.0
142.90	1264.0
144.10	138.0
146.60	162.0
147.60	216.0
155.00	222.0
156.90	176.0
158.80	153.0
172.10	185.0
174.00	62392.0
175.00	4514.0
176.00	62272.0
176.90	4256.0
177.80	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	1509.0
37.00	7510.0
38.00	6192.0
39.00	2659.0
39.90	450.0
41.80	159.0
43.00	231.0
44.00	2153.0
45.00	1497.0
46.90	1570.0
48.00	722.0
49.00	5704.0
50.00	21944.0
51.00	6209.0
51.90	492.0
52.80	124.0
54.90	474.0
56.00	2014.0
57.00	3194.0
57.90	256.0
59.90	971.0
61.00	4935.0
62.00	5437.0
63.00	3971.0
63.90	436.0
67.00	263.0
68.00	10340.0
69.00	11518.0
70.00	1013.0
71.90	506.0
73.10	4834.0
74.00	16480.0
75.00	49328.0
76.00	4107.0
77.10	691.0
78.90	4352.0
79.90	1206.0
81.00	4676.0
81.90	1089.0
82.80	124.0
86.90	3357.0
87.90	3658.0
91.00	482.0
92.00	2766.0
93.00	4561.0
94.00	11442.0
95.00	86288.0
96.00	5117.0
96.90	258.0
99.90	108.0
103.80	327.0
104.90	258.0
106.00	532.0
107.00	150.0
115.90	507.0
117.00	696.0
117.90	390.0
118.90	477.0
127.80	562.0
128.70	195.0
130.00	413.0
131.00	130.0
134.70	119.0
136.80	243.0
140.00	191.0
140.90	1265.0
141.90	152.0
143.00	1130.0
144.10	100.0
147.60	197.0
155.00	253.0
156.90	278.0
158.90	125.0
160.80	163.0
171.20	108.0
172.10	299.0
174.00	61352.0
175.00	4317.0
176.00	60824.0
176.90	3856.0
177.90	214.0
295.10	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34