


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU091924\
Data File : VU060886.D
Acq On : 19 Sep 2024 09:30
Operator : MD/SY
Sample : BFB001
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB001

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Sep 21 01:39:49 2024

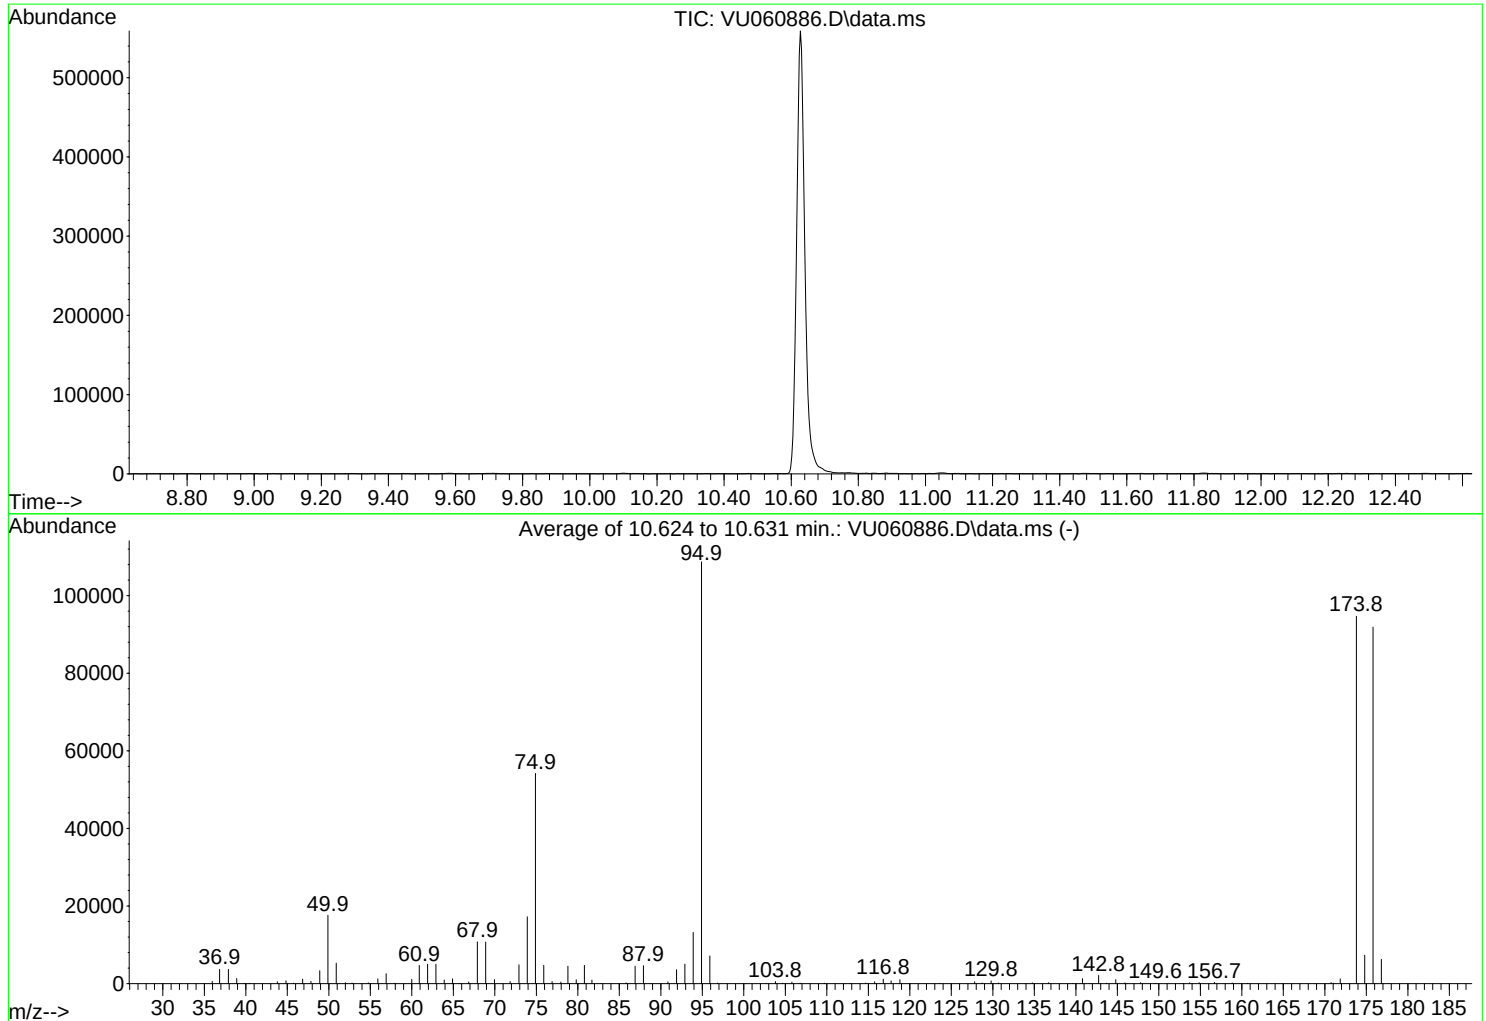

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	17608	PASS
75	95	30	80	49.8	54176	PASS
95	95	100	100	100.0	108728	PASS
96	95	5	9	6.6	7146	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.1	94709	PASS
175	174	5	9	7.7	7313	PASS
176	174	95	101	97.0	91888	PASS
177	176	5	9	6.8	6258	PASS

m/z	Abundance
39.70	110.0
43.80	221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
36.00	569.0
36.80	3531.0
37.90	3802.0
38.90	1317.0
39.90	160.0
40.50	103.0
43.80	765.0
44.80	704.0
45.80	128.0
46.80	1142.0
47.90	535.0
48.90	3486.0
49.90	17384.0
50.90	4926.0
52.00	284.0
52.80	115.0
54.80	222.0
55.90	1203.0
56.90	2433.0
58.00	137.0
60.00	1044.0
60.90	4639.0
61.90	5163.0
62.90	5021.0
63.90	1034.0
64.90	1372.0
66.80	370.0
67.90	10675.0
68.90	10504.0
69.90	988.0
71.80	564.0
72.90	4782.0
73.90	17160.0
74.90	53472.0
75.90	4712.0
76.90	495.0
77.90	455.0
78.80	4514.0
79.80	1082.0
80.80	4761.0
81.70	971.0
85.80	185.0
86.90	4272.0
87.90	4513.0
90.80	466.0
91.90	3565.0
92.90	5070.0
93.90	13344.0
94.90	106648.0
95.90	6748.0
97.00	162.0
103.80	512.0
104.70	132.0
105.80	379.0
106.80	158.0
109.70	107.0
114.80	133.0
115.80	439.0
116.80	1286.0
117.70	694.0
118.80	977.0
123.60	104.0
127.80	502.0
128.70	211.0
129.80	614.0
130.70	126.0
134.80	197.0
136.60	241.0
139.60	104.0
140.80	1194.0
141.70	170.0
142.70	1897.0
143.70	204.0
144.80	1080.0
145.90	238.0
147.80	281.0
149.60	152.0
153.70	197.0
154.80	285.0
156.70	359.0
158.90	180.0
160.70	149.0
170.70	474.0
171.80	1231.0
173.80	90560.0
174.80	7040.0
175.80	88648.0
176.80	6233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	594.0
36.90	3785.0
37.90	3800.0
38.90	1367.0
39.90	223.0
40.50	111.0
43.80	709.0
44.90	729.0
45.80	136.0
46.80	1230.0
47.90	611.0
48.90	3417.0
49.90	18280.0
50.90	5373.0
52.00	256.0
52.80	183.0
54.70	218.0
55.90	1233.0
56.90	2622.0
58.00	122.0
60.00	1211.0
60.90	4824.0
61.90	5118.0
62.90	5228.0
63.90	978.0
64.90	1274.0
65.80	114.0
66.80	425.0
67.90	11188.0
68.90	11194.0
69.90	1129.0
71.80	547.0
72.90	4971.0
73.90	17600.0
74.90	55928.0
75.90	4905.0
76.90	528.0
77.90	411.0
78.80	4658.0
79.80	1010.0
80.80	4850.0
81.70	944.0
85.80	226.0
86.90	4629.0
87.90	4908.0
90.90	430.0
91.90	3770.0
92.90	5161.0
93.90	13584.0
94.90	112248.0
95.90	7442.0
96.80	169.0
103.80	573.0
104.60	138.0
105.80	397.0
106.80	157.0
109.70	140.0
112.90	104.0
114.70	144.0
115.80	530.0
116.80	1173.0
117.70	716.0
118.80	1087.0
123.60	116.0
127.80	526.0
128.70	198.0
129.80	762.0
130.70	168.0
134.70	210.0
136.70	268.0
140.80	1311.0
141.70	128.0
142.70	2189.0
143.70	163.0
144.80	1068.0
145.90	195.0
147.80	273.0
149.60	125.0
153.70	218.0
154.90	282.0
156.70	319.0
158.80	141.0
160.70	113.0
170.80	394.0
171.90	1268.0
173.80	97888.0
174.80	7495.0
175.80	94704.0
176.80	6431.0
177.70	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001

m/z	Abundance
35.90	549.0
36.90	3770.0
37.90	3353.0
38.90	1345.0
39.90	217.0
40.40	101.0
43.80	728.0
44.90	757.0
45.70	133.0
46.90	1150.0
47.80	595.0
48.90	3151.0
49.90	17160.0
50.90	5540.0
52.00	194.0
52.80	199.0
54.70	195.0
55.90	1262.0
56.90	2617.0
57.90	102.0
60.00	1089.0
60.90	4630.0
61.90	4738.0
62.90	4786.0
63.90	855.0
64.90	1127.0
65.80	146.0
66.90	421.0
67.90	10479.0
68.90	10511.0
70.00	1035.0
71.90	546.0
72.90	4798.0
73.90	16920.0
74.90	53128.0
75.90	4439.0
76.90	574.0
78.00	423.0
78.80	4330.0
79.80	915.0
80.80	4483.0
81.70	875.0
82.80	109.0
85.80	181.0
86.90	4565.0
87.90	4451.0
88.70	103.0
90.90	415.0
91.90	3499.0
92.90	4881.0
93.90	12728.0
94.90	107288.0
95.90	7249.0
96.80	185.0
102.70	103.0
103.80	532.0
104.80	113.0
105.80	431.0
106.80	127.0
109.70	102.0
112.90	112.0
114.60	222.0
115.70	506.0
116.80	968.0
117.80	681.0
118.80	1001.0
127.80	479.0
128.70	138.0
129.80	776.0
130.70	175.0
134.70	229.0
136.80	279.0
140.80	1297.0
142.80	2220.0
144.80	999.0
145.90	146.0
147.80	215.0
152.90	109.0
153.70	191.0
154.90	213.0
156.70	277.0
158.80	123.0
171.00	372.0
171.90	1222.0
173.80	95680.0
174.80	7405.0
175.80	92312.0
176.80	6111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB001