


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092018\
Data File : VU026897.D
Acq On : 19 Sep 2018 14:31
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U091218W.M
Title : SW846 8260
Last Update : Fri Sep 21 16:48:15 2018

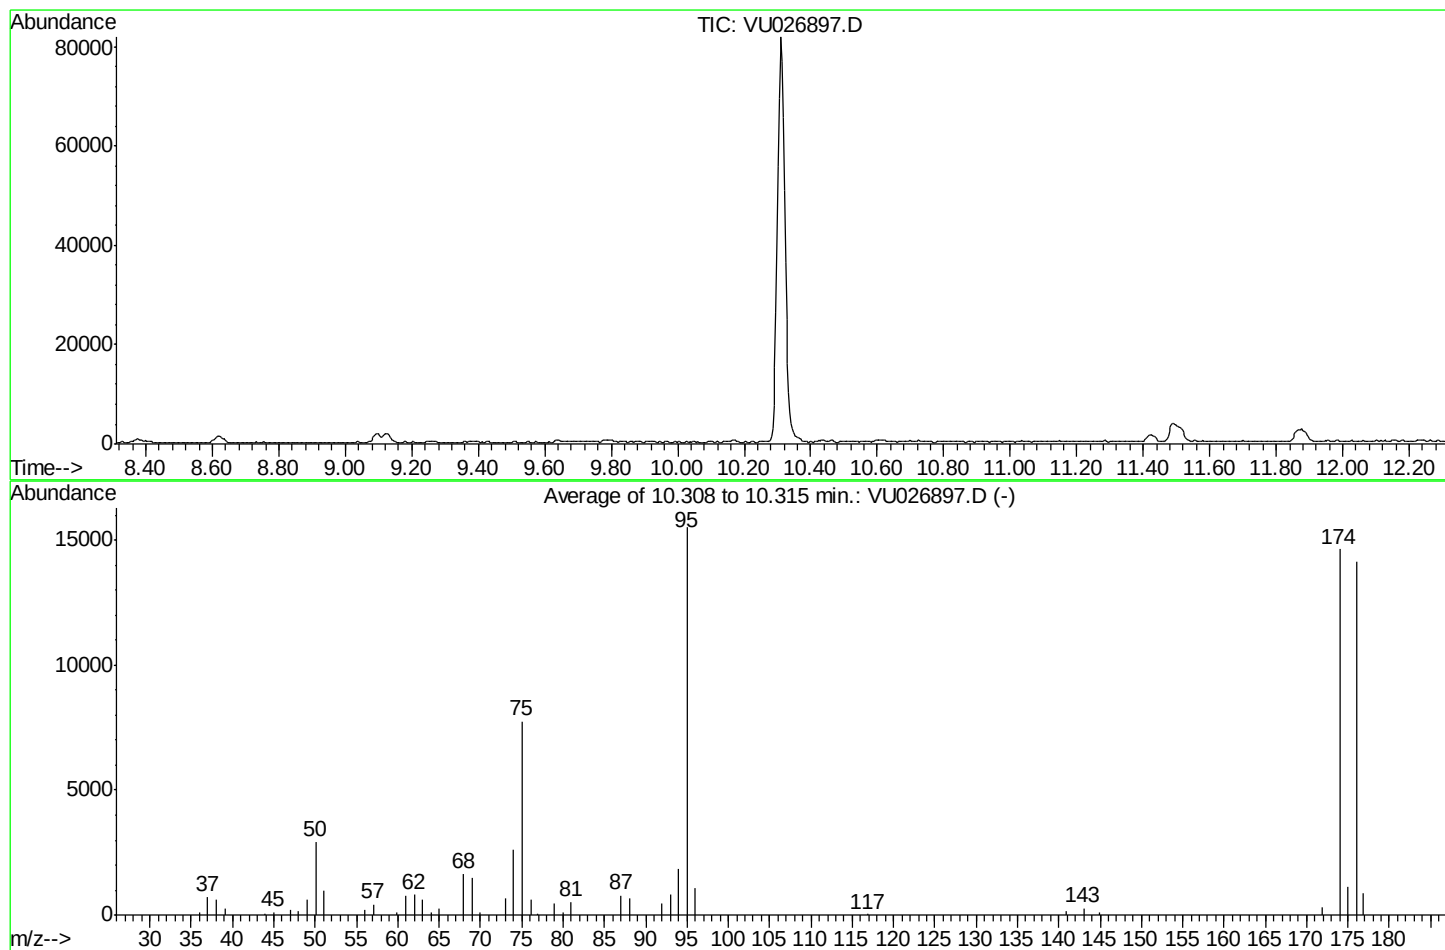

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	2933	PASS
75	95	30	60	50.0	7758	PASS
95	95	100	100	100.0	15526	PASS
96	95	5	9	6.9	1072	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	94.4	14657	PASS
175	174	5	9	7.7	1122	PASS
176	174	95	101	96.6	14163	PASS
177	176	5	9	6.2	885	PASS