

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Quantitation Report (QT Reviewed)


Data File : VU034683.D
Acq On : 20 Sep 2019 13:01
Operator : JC/SP
Sample : K4895-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BDF5

Manual Integrations
APPROVED

MMDadoda
9/23/2019 9:32:49 AM

Quant Time: Sep 21 03:30:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 21 02:29:10 2019
Response via : Initial Calibration

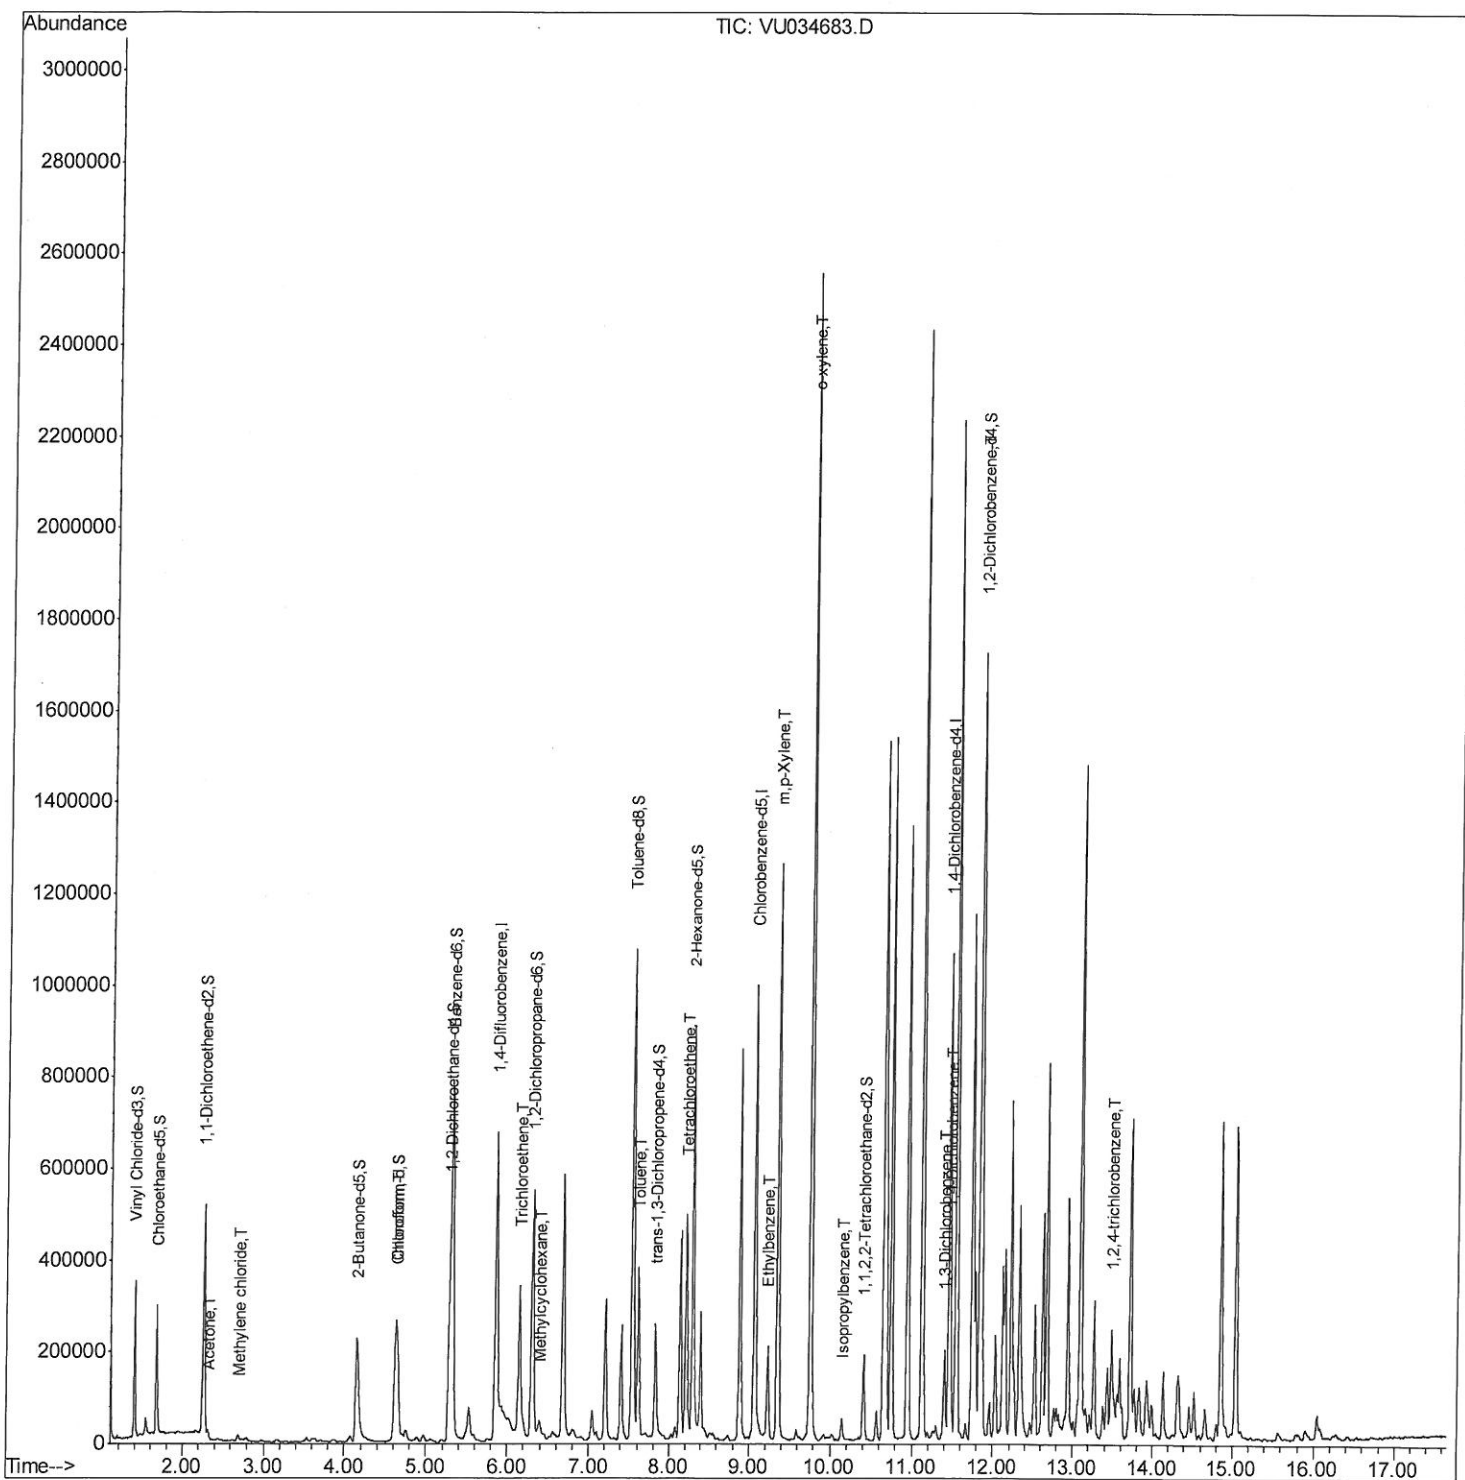

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Quantitation Report (Qedit)




Data File : VU034683.D
Acq On : 20 Sep 2019 13:01
Operator : JC/SP
Sample : K4895-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDF5

Manual Integrations
APPROVED

MMDadoda
9/23/2019 9:32:49 AM

Quant Time: Sep 21 02:32:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 21 02:29:10 2019
Response via : Initial Calibration

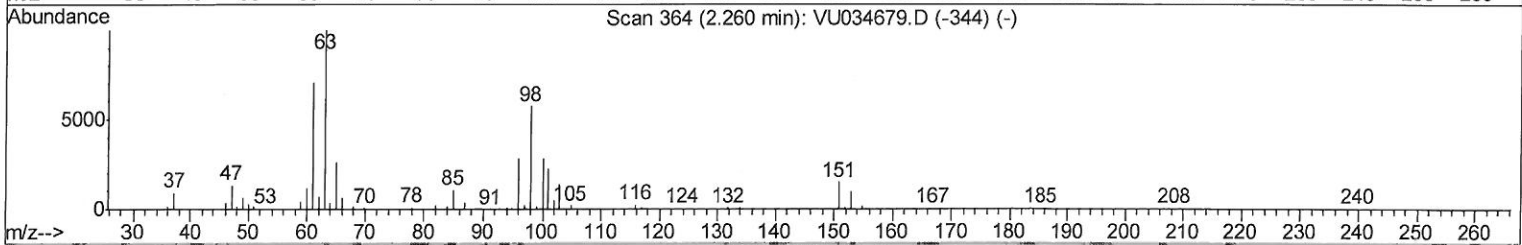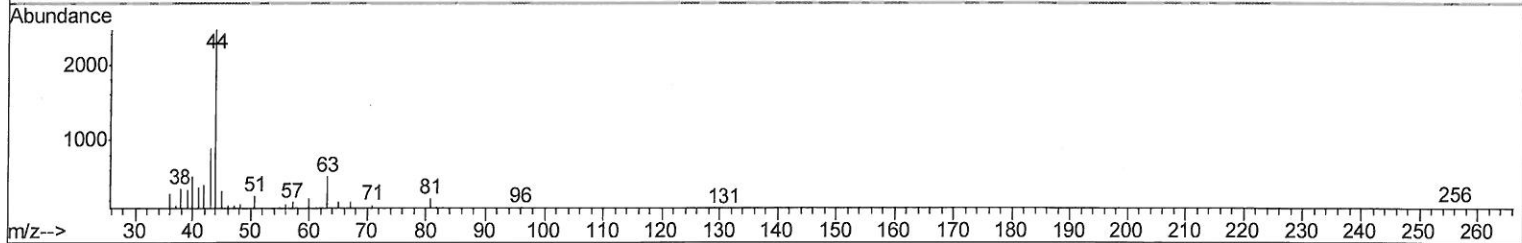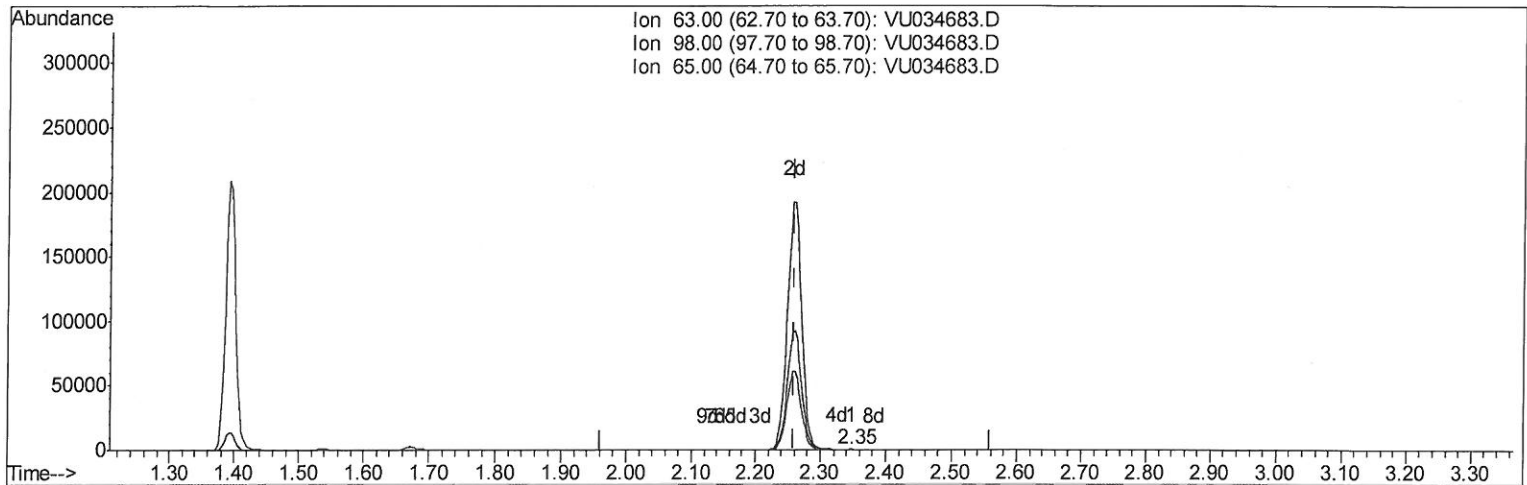

TIC: VU034683.D

(11) 1,1-Dichloroethene-d2 (S)

2.347min (+0.087) 0.04ug/L

response 332

Ion	Exp%	Act%
63.00	100	100
98.00	57.60	57.23
65.00	24.00	30.42
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Quantitation Report (Qedit)




Data File : VU034683.D
Acq On : 20 Sep 2019 13:01
Operator : JC/SP
Sample : K4895-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDF5

Manual Integrations
APPROVED

MMDadoda
9/23/2019 9:32:49 AM

Quant Time: Sep 21 02:32:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 21 02:29:10 2019
Response via : Initial Calibration

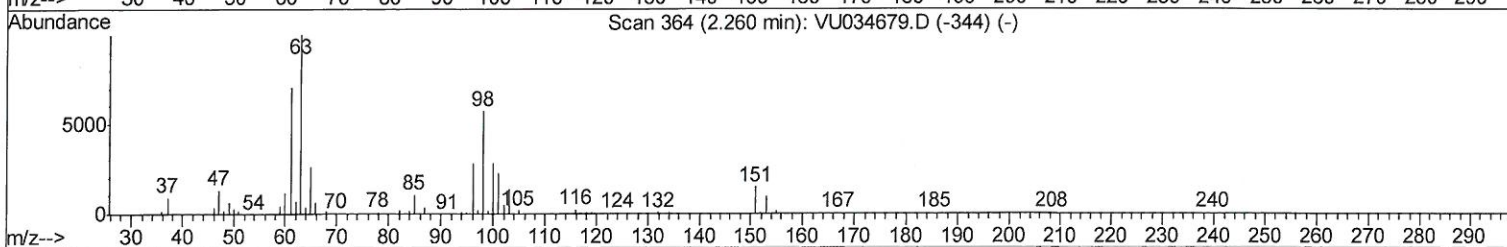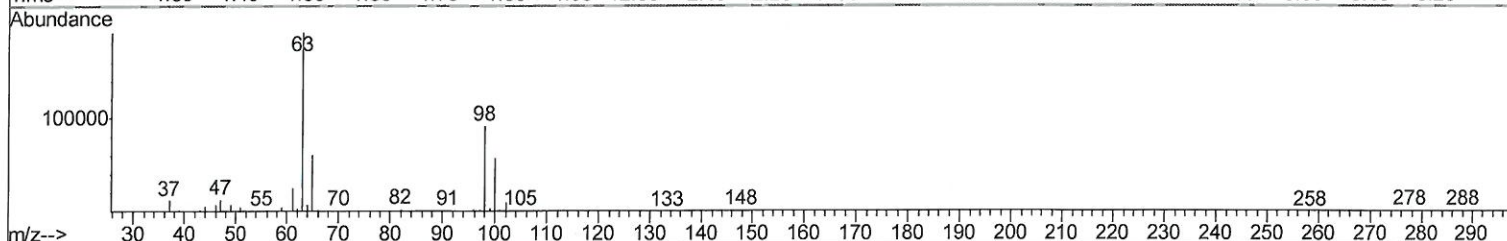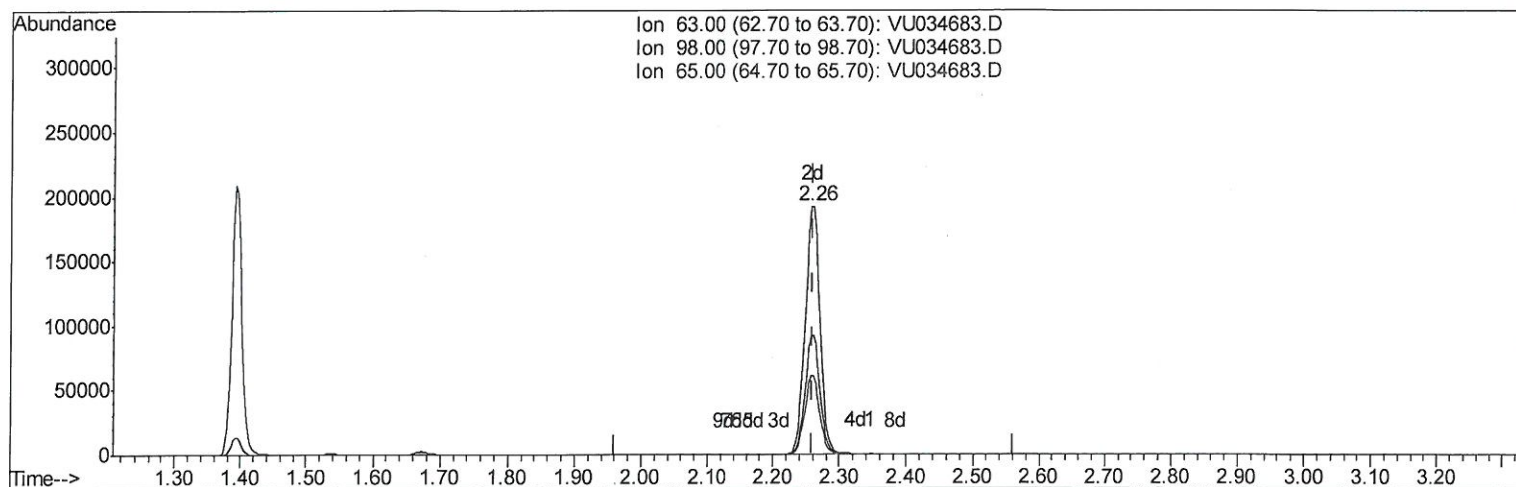

TIC: VU034683.D

(11) 1,1-Dichloroethene-d2 (S)

2.257min (-0.003) 34.74ug/L m

response 295137

Ion	Exp%	Act%
63.00	100	100
98.00	57.60	0.06#
65.00	24.00	0.03#
0.00	0.00	0.00

7M0
9/30/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Quantitation Report (QT Reviewed)

Data File : VU034683.D
Acq On : 20 Sep 2019 13:01
Operator : JC/SP
Sample : K4895-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDF5

Manual Integrations
APPROVED

MMDadoda
9/23/2019 9:32:49 AM

Quant Time: Sep 21 03:30:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 21 02:29:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	489989	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	467068	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	225360	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	221373	44.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.26%
7) Chloroethane-d5	1.67	69	178980	46.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.34%
11) 1,1-Dichloroethene-d2	2.26	63	295137m	34.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.48%
21) 2-Butanone-d5	4.15	46	369848	96.20	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.20%
24) Chloroform-d	4.62	84	192567	26.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	52.82%#
26) 1,2-Dichloroethane-d4	5.29	65	258465	48.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.42%
32) Benzene-d6	5.32	84	698339	48.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.48%
36) 1,2-Dichloropropane-d6	6.31	67	249046	49.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.44%
41) Toluene-d8	7.54	98	667060	48.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.86%
43) trans-1,3-Dichloropropene-	7.83	79	109998	45.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.78%
47) 2-Hexanone-d5	8.29	63	250217	98.46	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.46%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	86866	12.37	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	24.74%#
64) 1,2-Dichlorobenzene-d4	11.84	152	233301	49.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.74%

7 MLO
9/30/19

Target Compounds

					Qvalue
13) Acetone	2.31	43	20952	4.685	ug/L 99
16) Methylene chloride	2.68	84	4356	1.073	ug/L 96
25) Chloroform	4.65	83	160470	20.267	ug/L 98
34) Trichloroethene	6.16	95	10025	2.506	ug/L # 85
35) Methylcyclohexane	6.39	83	11211	1.651	ug/L 95
42) Toluene	7.61	91	252275	14.410	ug/L 97
46) Tetrachloroethene	8.21	164	90560	32.181	ug/L 94
52) Ethylbenzene	9.23	91	139583	7.080	ug/L 100
53) m,p-Xylene	9.35	106	318974	45.681	ug/L 96
54) o-xylene	9.76	106	590091	85.441	ug/L 96
56) Isopropylbenzene	10.14	105	28127	1.510	ug/L 95
62) 1,3-Dichlorobenzene	11.40	146	12707	1.628	ug/L 90
63) 1,4-Dichlorobenzene	11.49	146	20660	2.599	ug/L 94
65) 1,2-Dichlorobenzene	11.85	146	209941	26.623	ug/L 98
68) 1,2,4-trichlorobenzene	13.48	180	7629	1.855	ug/L # 69

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Quantitation Report (QT Reviewed)

Data File : VU034683.D
Acq On : 20 Sep 2019 13:01
Operator : JC/SP
Sample : K4895-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDF5

Manual Integrations
APPROVED

MMDadoda
9/23/2019 9:32:49 AM

Quant Time: Sep 21 03:30:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Sep 21 02:29:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev	(Min)
--------------------	------	------	----------	------	-------	-----	-------

(#) = qualifier out of range (m) = manual integration (+) = signals summed