

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034685.D
 Acq On : 20 Sep 2019 13:47
 Operator : JC/SP
 Sample : K4982-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	87	95	107	rBV	339794	358939	15.08%	1.976%
2	1.672	174	181	196	rVB	270679	338870	14.24%	1.866%
3	2.257	354	363	374	rBV	483536	723169	30.39%	3.982%
4	2.431	410	417	426	rVB	14018	22125	0.93%	0.122%
5	2.907	562	565	570	rVB5	1498	1282	0.05%	0.007%
6	3.026	598	602	607	rVB6	2248	1977	0.08%	0.011%
7	3.068	609	615	616	rBV2	901	830	0.03%	0.005%
8	3.080	616	619	621	rBV3	1692	975	0.04%	0.005%
9	3.174	644	648	650	rBV4	1207	795	0.03%	0.004%
10	3.241	663	669	674	rVB8	863	964	0.04%	0.005%
11	3.270	674	678	680	rBV4	1930	1101	0.05%	0.006%
12	3.450	732	734	738	rVV5	999	793	0.03%	0.004%
13	3.479	741	743	751	rVV7	933	939	0.04%	0.005%
14	3.576	767	773	776	rBV6	1816	1829	0.08%	0.010%
15	3.633	784	791	794	rVV6	1841	2300	0.10%	0.013%
16	3.704	810	813	816	rVV3	1233	925	0.04%	0.005%
17	3.717	816	817	820	rVB2	2049	829	0.03%	0.005%
18	3.740	820	824	826	rBV3	1522	1293	0.05%	0.007%
19	3.884	866	869	875	rBV7	1187	1060	0.04%	0.006%
20	3.916	875	879	880	rBV3	1620	1029	0.04%	0.006%
21	4.016	905	910	915	rBV7	905	827	0.03%	0.005%
22	4.064	920	925	930	rBV7	1798	2063	0.09%	0.011%
23	4.096	932	935	937	rVB3	1588	899	0.04%	0.005%
24	4.151	937	952	979	rBV	228920	642751	27.01%	3.539%
25	4.418	1033	1035	1040	rVB4	2049	1028	0.04%	0.006%
26	4.502	1058	1061	1064	rBV4	1200	769	0.03%	0.004%
27	4.521	1064	1067	1070	rVB3	1480	1016	0.04%	0.006%
28	4.543	1070	1074	1075	rBV2	1427	970	0.04%	0.005%
29	4.624	1081	1099	1128	rBV	376815	909369	38.22%	5.007%
30	4.926	1187	1193	1196	rBV8	1409	1900	0.08%	0.010%
31	5.042	1224	1229	1230	rBV4	1103	971	0.04%	0.005%
32	5.177	1267	1271	1273	rBV3	1575	1054	0.04%	0.006%
33	5.209	1278	1281	1285	rVB3	2050	1407	0.06%	0.008%
34	5.315	1290	1314	1343	rBV2	766000	2379611	100.00%	13.102%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034685.D
 Acq On : 20 Sep 2019 13:47
 Operator : JC/SP
 Sample : K4982-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	5.540	1380	1384	1388	rBV7	1665	1380	0.06%	0.008%
36	5.865	1470	1485	1503	rBV	654350	1447268	60.82%	7.969%
37	6.309	1610	1623	1642	rBV	535011	1064019	44.71%	5.858%
38	7.128	1874	1878	1886	rVB7	2209	2602	0.11%	0.014%
39	7.206	1889	1902	1925	rBV	320835	602118	25.30%	3.315%
40	7.543	1994	2007	2022	rBV	1027670	1802048	75.73%	9.922%
41	7.617	2023	2030	2049	rVB	86121	164478	6.91%	0.906%
42	7.829	2085	2096	2122	rBV2	218061	399653	16.79%	2.200%
43	8.058	2165	2167	2172	rVB5	1353	1089	0.05%	0.006%
44	8.087	2173	2176	2179	rBV4	2251	1305	0.05%	0.007%
45	8.151	2190	2196	2203	rBV6	5401	7633	0.32%	0.042%
46	8.209	2208	2214	2226	rVB4	14142	22242	0.93%	0.122%
47	8.289	2228	2239	2278	rBV	714454	1385109	58.21%	7.626%
48	8.505	2302	2306	2310	rVB7	2154	1873	0.08%	0.010%
49	8.649	2347	2351	2352	rBV3	1199	916	0.04%	0.005%
50	8.752	2381	2383	2389	rVB7	1918	1191	0.05%	0.007%
51	8.833	2405	2408	2412	rBV5	1196	1036	0.04%	0.006%
52	9.067	2467	2481	2510	rBV	915912	1587676	66.72%	8.742%
53	9.231	2526	2532	2543	rVB5	9644	15266	0.64%	0.084%
54	9.292	2549	2551	2556	rBV5	1449	822	0.03%	0.005%
55	9.357	2561	2571	2584	rBV2	33338	63159	2.65%	0.348%
56	9.469	2602	2606	2608	rBV5	1419	1168	0.05%	0.006%
57	9.678	2668	2671	2674	rVB4	1773	1006	0.04%	0.006%
58	9.697	2674	2677	2679	rBV2	1334	974	0.04%	0.005%
59	9.762	2689	2697	2713	rVB3	23643	39532	1.66%	0.218%
60	10.029	2777	2780	2784	rBV5	2165	1819	0.08%	0.010%
61	10.087	2795	2798	2801	rVB4	1894	1109	0.05%	0.006%
62	10.212	2833	2837	2841	rBV6	2676	2191	0.09%	0.012%
63	10.279	2855	2858	2860	rBV3	1582	1156	0.05%	0.006%
64	10.312	2866	2868	2874	rVB4	1719	1448	0.06%	0.008%
65	10.408	2885	2898	2923	rBV	678430	1118988	47.02%	6.161%
66	10.569	2944	2948	2949	rBV4	2941	1757	0.07%	0.010%
67	10.588	2950	2954	2963	rVB7	7962	10905	0.46%	0.060%
68	10.665	2964	2978	2985	rBV8	8754	19012	0.80%	0.105%
69	10.842	3030	3033	3035	rBV2	1431	968	0.04%	0.005%
70	10.919	3054	3057	3060	rVB5	1587	1098	0.05%	0.006%
71	10.948	3060	3066	3076	rBV9	5081	8442	0.35%	0.046%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034685.D
 Acq On : 20 Sep 2019 13:47
 Operator : JC/SP
 Sample : K4982-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	10.993	3076	3080	3083	rBV6	1229	1094	0.05%	0.006%
73	11.054	3096	3099	3102	rBV5	1363	944	0.04%	0.005%
74	11.132	3115	3123	3132	rVB2	16363	24549	1.03%	0.135%
75	11.305	3173	3177	3182	rVB8	1130	1107	0.05%	0.006%
76	11.350	3187	3191	3192	rBV3	1334	866	0.04%	0.005%
77	11.376	3196	3199	3200	rBV4	1528	878	0.04%	0.005%
78	11.459	3213	3225	3247	rBV	842797	1395309	58.64%	7.683%
79	11.836	3330	3342	3362	rBV	899589	1508305	63.38%	8.305%
80	12.209	3455	3458	3461	rBV5	2335	1829	0.08%	0.010%
81	12.620	3581	3586	3588	rBV5	2859	2600	0.11%	0.014%
82	12.688	3604	3607	3612	rVB6	2745	2321	0.10%	0.013%
83	12.848	3655	3657	3660	rVB3	1750	775	0.03%	0.004%
84	12.877	3660	3666	3672	rBV10	2840	4318	0.18%	0.024%
85	12.932	3681	3683	3685	rBV3	1788	1149	0.05%	0.006%
86	13.109	3733	3738	3744	rBV8	3802	5035	0.21%	0.028%
87	13.164	3752	3755	3758	rBV5	1383	1205	0.05%	0.007%
88	13.218	3769	3772	3776	rBV5	1251	1078	0.05%	0.006%
89	13.344	3808	3811	3814	rVB7	1493	763	0.03%	0.004%
90	13.363	3814	3817	3820	rBV4	2137	1980	0.08%	0.011%
91	13.424	3834	3836	3841	rBV3	1621	1387	0.06%	0.008%
92	13.485	3850	3855	3856	rBV4	1769	1452	0.06%	0.008%
93	13.556	3873	3877	3882	rBV8	1816	1924	0.08%	0.011%
94	13.607	3891	3893	3897	rVB4	1915	1175	0.05%	0.006%
95	13.710	3923	3925	3926	rBV2	1557	819	0.03%	0.005%
96	13.739	3931	3934	3936	rBV4	3919	3074	0.13%	0.017%
97	13.807	3953	3955	3957	rBV3	1967	802	0.03%	0.004%
98	14.106	4045	4048	4052	rVB4	2582	1855	0.08%	0.010%
99	14.128	4052	4055	4058	rBV4	1738	1182	0.05%	0.007%
100	14.569	4189	4192	4195	rBV4	1926	1082	0.05%	0.006%


Sum of corrected areas: 18161972

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034685.D
Acq On : 20 Sep 2019 13:47
Operator : JC/SP
Sample : K4982-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

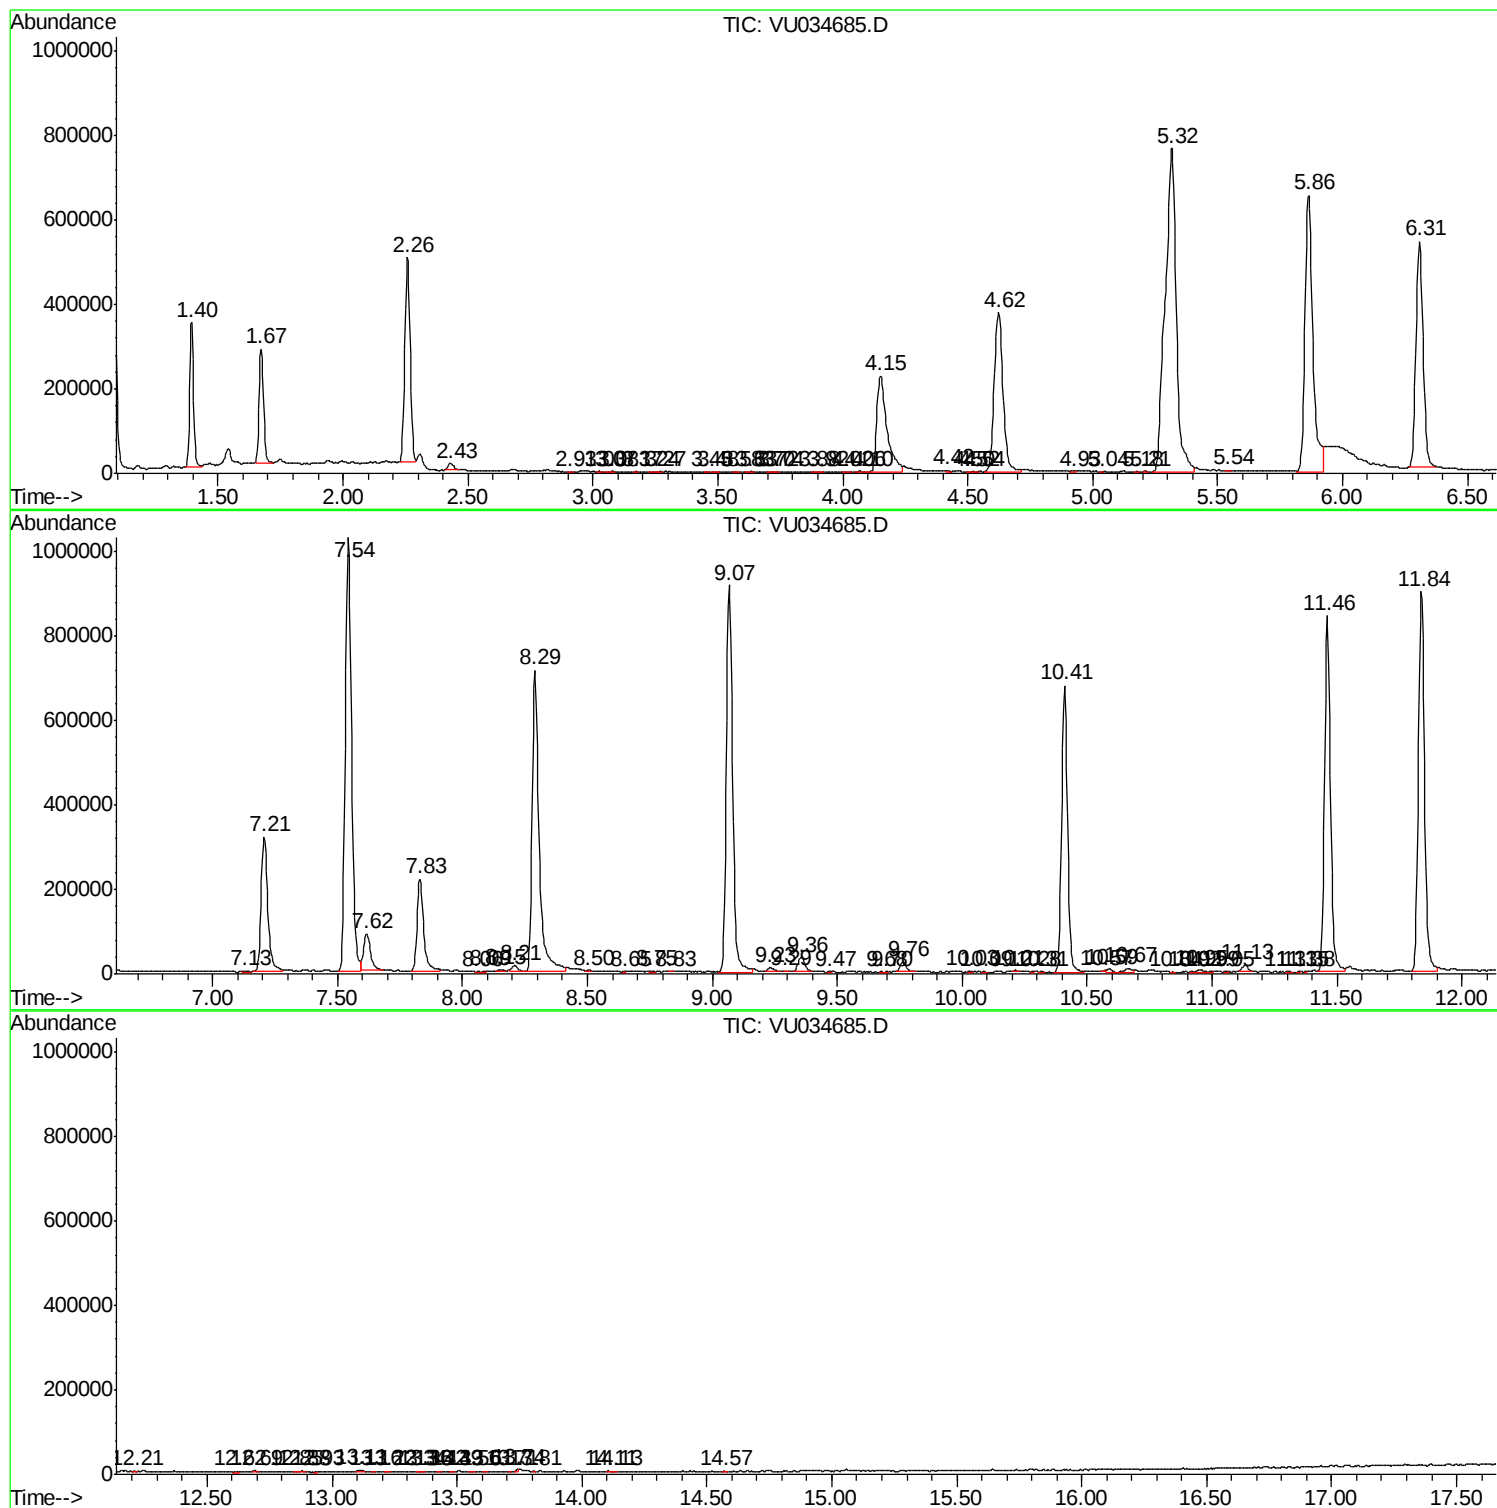

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034685.D
Acq On : 20 Sep 2019 13:47
Operator : JC/SP
Sample : K4982-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AT7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU092019\
Data File : VU034685.D
Acq On : 20 Sep 2019 13:47
Operator : JC/SP
Sample : K4982-01
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0AT7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc