

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034692.D
 Acq On : 20 Sep 2019 16:31
 Operator : JC/SP
 Sample : K4948-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	21	27	33	rBV	45791	43378	1.43%	0.202%
2	1.392	87	94	108	rBV	349698	369036	12.16%	1.715%
3	1.672	174	181	195	rVB	281651	351699	11.59%	1.634%
4	2.257	354	363	377	rVB	494996	765056	25.21%	3.555%
5	2.428	408	416	429	rBV	41828	70103	2.31%	0.326%
6	2.563	455	458	459	rBV2	1456	860	0.03%	0.004%
7	2.627	474	478	480	rBV4	2121	1695	0.06%	0.008%
8	2.685	494	496	500	rVB5	2118	1316	0.04%	0.006%
9	2.926	568	571	573	rBV2	1615	858	0.03%	0.004%
10	2.978	576	587	603	rBV2	16139	35508	1.17%	0.165%
11	3.113	623	629	634	rVB9	1211	1590	0.05%	0.007%
12	3.203	655	657	661	rVB5	1401	776	0.03%	0.004%
13	3.325	692	695	699	rVB4	1098	933	0.03%	0.004%
14	3.379	709	712	716	rBV7	1027	761	0.03%	0.004%
15	3.524	754	757	759	rVV4	1790	1206	0.04%	0.006%
16	3.559	766	768	774	rVB6	1494	1248	0.04%	0.006%
17	3.588	774	777	779	rBV4	1028	802	0.03%	0.004%
18	3.604	780	782	787	rVB4	1649	1045	0.03%	0.005%
19	3.633	787	791	793	rBV3	1590	1058	0.03%	0.005%
20	3.672	802	803	806	rVB	1482	670	0.02%	0.003%
21	3.691	806	809	811	rBV3	1297	812	0.03%	0.004%
22	3.704	811	813	815	rVV3	1399	928	0.03%	0.004%
23	3.727	818	820	823	rVB3	1478	830	0.03%	0.004%
24	3.781	835	837	841	rVB4	1821	1186	0.04%	0.006%
25	3.810	841	846	850	rBV5	1995	2146	0.07%	0.010%
26	3.833	850	853	855	rBV	1482	893	0.03%	0.004%
27	3.852	855	859	862	rBV4	1356	1222	0.04%	0.006%
28	4.032	912	915	919	rBV4	1235	735	0.02%	0.003%
29	4.064	923	925	930	rVB6	1118	637	0.02%	0.003%
30	4.090	930	933	937	rBV5	2182	1686	0.06%	0.008%
31	4.151	940	952	960	rBV	231147	545372	17.97%	2.534%
32	4.492	1055	1058	1061	rBV5	1809	1094	0.04%	0.005%
33	4.556	1074	1078	1080	rBV4	1253	1028	0.03%	0.005%
34	4.621	1082	1098	1123	rVV	384897	913041	30.08%	4.242%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034692.D
 Acq On : 20 Sep 2019 16:31
 Operator : JC/SP
 Sample : K4948-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	4.801	1152	1154	1159	rVB5	3070	2148	0.07%	0.010%
36	4.990	1210	1213	1222	rVB8	1943	2730	0.09%	0.013%
37	5.032	1222	1226	1230	rBV6	2023	2160	0.07%	0.010%
38	5.071	1235	1238	1239	rVV2	1330	771	0.03%	0.004%
39	5.096	1243	1246	1248	rVV3	1106	678	0.02%	0.003%
40	5.109	1248	1250	1254	rVB4	2056	1078	0.04%	0.005%
41	5.135	1254	1258	1260	rBV5	1163	850	0.03%	0.004%
42	5.315	1289	1314	1343	rBV2	791962	2377106	78.32%	11.045%
43	5.646	1414	1417	1419	rBV3	1463	852	0.03%	0.004%
44	5.678	1424	1427	1433	rBV6	2315	2349	0.08%	0.011%
45	5.865	1468	1485	1503	rBV	691319	1511857	49.81%	7.025%
46	6.164	1570	1578	1598	rVB2	94472	193078	6.36%	0.897%
47	6.309	1609	1623	1645	rVB	545830	1102787	36.33%	5.124%
48	6.707	1745	1747	1753	rBV6	1578	1286	0.04%	0.006%
49	7.010	1838	1841	1844	rBV5	2342	1391	0.05%	0.006%
50	7.116	1872	1874	1878	rVB4	1883	946	0.03%	0.004%
51	7.138	1878	1881	1882	rBV3	1206	779	0.03%	0.004%
52	7.206	1890	1902	1922	rBV	326717	610999	20.13%	2.839%
53	7.489	1985	1990	1993	rBV6	1575	1800	0.06%	0.008%
54	7.543	1994	2007	2031	rBV	1057080	1863268	61.39%	8.658%
55	7.710	2057	2059	2062	rBV2	1794	1060	0.03%	0.005%
56	7.829	2084	2096	2114	rBV2	218083	401139	13.22%	1.864%
57	8.206	2195	2213	2229	rBV	1772750	3035057	100.00%	14.102%
58	8.289	2229	2239	2268	rVB	734655	1349267	44.46%	6.269%
59	8.826	2404	2406	2407	rBV2	1517	637	0.02%	0.003%
60	8.849	2410	2413	2417	rBV6	1764	1534	0.05%	0.007%
61	8.887	2422	2425	2430	rVB5	2720	1878	0.06%	0.009%
62	8.910	2430	2432	2435	rBV3	1851	1423	0.05%	0.007%
63	8.964	2445	2449	2452	rVB5	1269	1023	0.03%	0.005%
64	9.067	2469	2481	2507	rVV	989443	1669565	55.01%	7.757%
65	9.263	2541	2542	2547	rBV5	1099	824	0.03%	0.004%
66	9.312	2553	2557	2559	rBV5	1245	993	0.03%	0.005%
67	9.353	2566	2570	2579	rBV9	3757	4982	0.16%	0.023%
68	9.418	2588	2590	2595	rBV5	1151	770	0.03%	0.004%
69	9.450	2596	2600	2602	rBV6	2060	1456	0.05%	0.007%
70	9.508	2614	2618	2622	rBV6	2396	2584	0.09%	0.012%
71	9.659	2662	2665	2669	rVB4	1725	1051	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092019\
 Data File : VU034692.D
 Acq On : 20 Sep 2019 16:31
 Operator : JC/SP
 Sample : K4948-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEDN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	9.688	2669	2674	2675	rBV4	1915	1288	0.04%	0.006%
73	9.759	2690	2696	2701	rBV9	3451	4402	0.15%	0.020%
74	9.813	2711	2713	2716	rVB3	1991	955	0.03%	0.004%
75	9.845	2716	2723	2726	rVB10	2364	2502	0.08%	0.012%
76	9.868	2726	2730	2731	rBV2	1394	840	0.03%	0.004%
77	9.916	2739	2745	2746	rBV4	2166	2078	0.07%	0.010%
78	9.961	2756	2759	2762	rBV3	1290	893	0.03%	0.004%
79	10.128	2808	2811	2812	rBV3	1750	994	0.03%	0.005%
80	10.279	2855	2858	2861	rBV5	2145	1486	0.05%	0.007%
81	10.408	2885	2898	2916	rBV	699083	1142416	37.64%	5.308%
82	10.582	2946	2952	2955	rBV7	3407	4106	0.14%	0.019%
83	10.669	2972	2979	2981	rBV6	2103	2158	0.07%	0.010%
84	10.730	2995	2998	3001	rBV5	2665	1762	0.06%	0.008%
85	10.839	3029	3032	3038	rVB9	1444	1377	0.05%	0.006%
86	10.906	3049	3053	3054	rBV3	1449	1178	0.04%	0.005%
87	10.929	3058	3060	3062	rBV3	1095	689	0.02%	0.003%
88	11.061	3095	3101	3104	rBV7	2360	2614	0.09%	0.012%
89	11.125	3119	3121	3123	rBV2	1873	1169	0.04%	0.005%
90	11.305	3171	3177	3179	rBV6	1771	2042	0.07%	0.009%
91	11.376	3195	3199	3202	rBV5	2120	2188	0.07%	0.010%
92	11.459	3213	3225	3248	rBV	905051	1495259	49.27%	6.948%
93	11.707	3298	3302	3307	rVB5	2745	2713	0.09%	0.013%
94	11.775	3320	3323	3324	rBV3	2567	1314	0.04%	0.006%
95	11.836	3330	3342	3366	rBV	926998	1558130	51.34%	7.240%
96	12.463	3534	3537	3540	rBV4	2941	2030	0.07%	0.009%
97	12.588	3573	3576	3578	rBV3	2342	1724	0.06%	0.008%
98	12.688	3602	3607	3609	rBV5	4385	4544	0.15%	0.021%
99	12.765	3629	3631	3634	rBV3	1980	1047	0.03%	0.005%
100	13.980	4006	4009	4010	rBV2	4340	2728	0.09%	0.013%


Sum of corrected areas: 21521990

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092019\
Data File : VU034692.D
Acq On : 20 Sep 2019 16:31
Operator : JC/SP
Sample : K4948-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDN5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

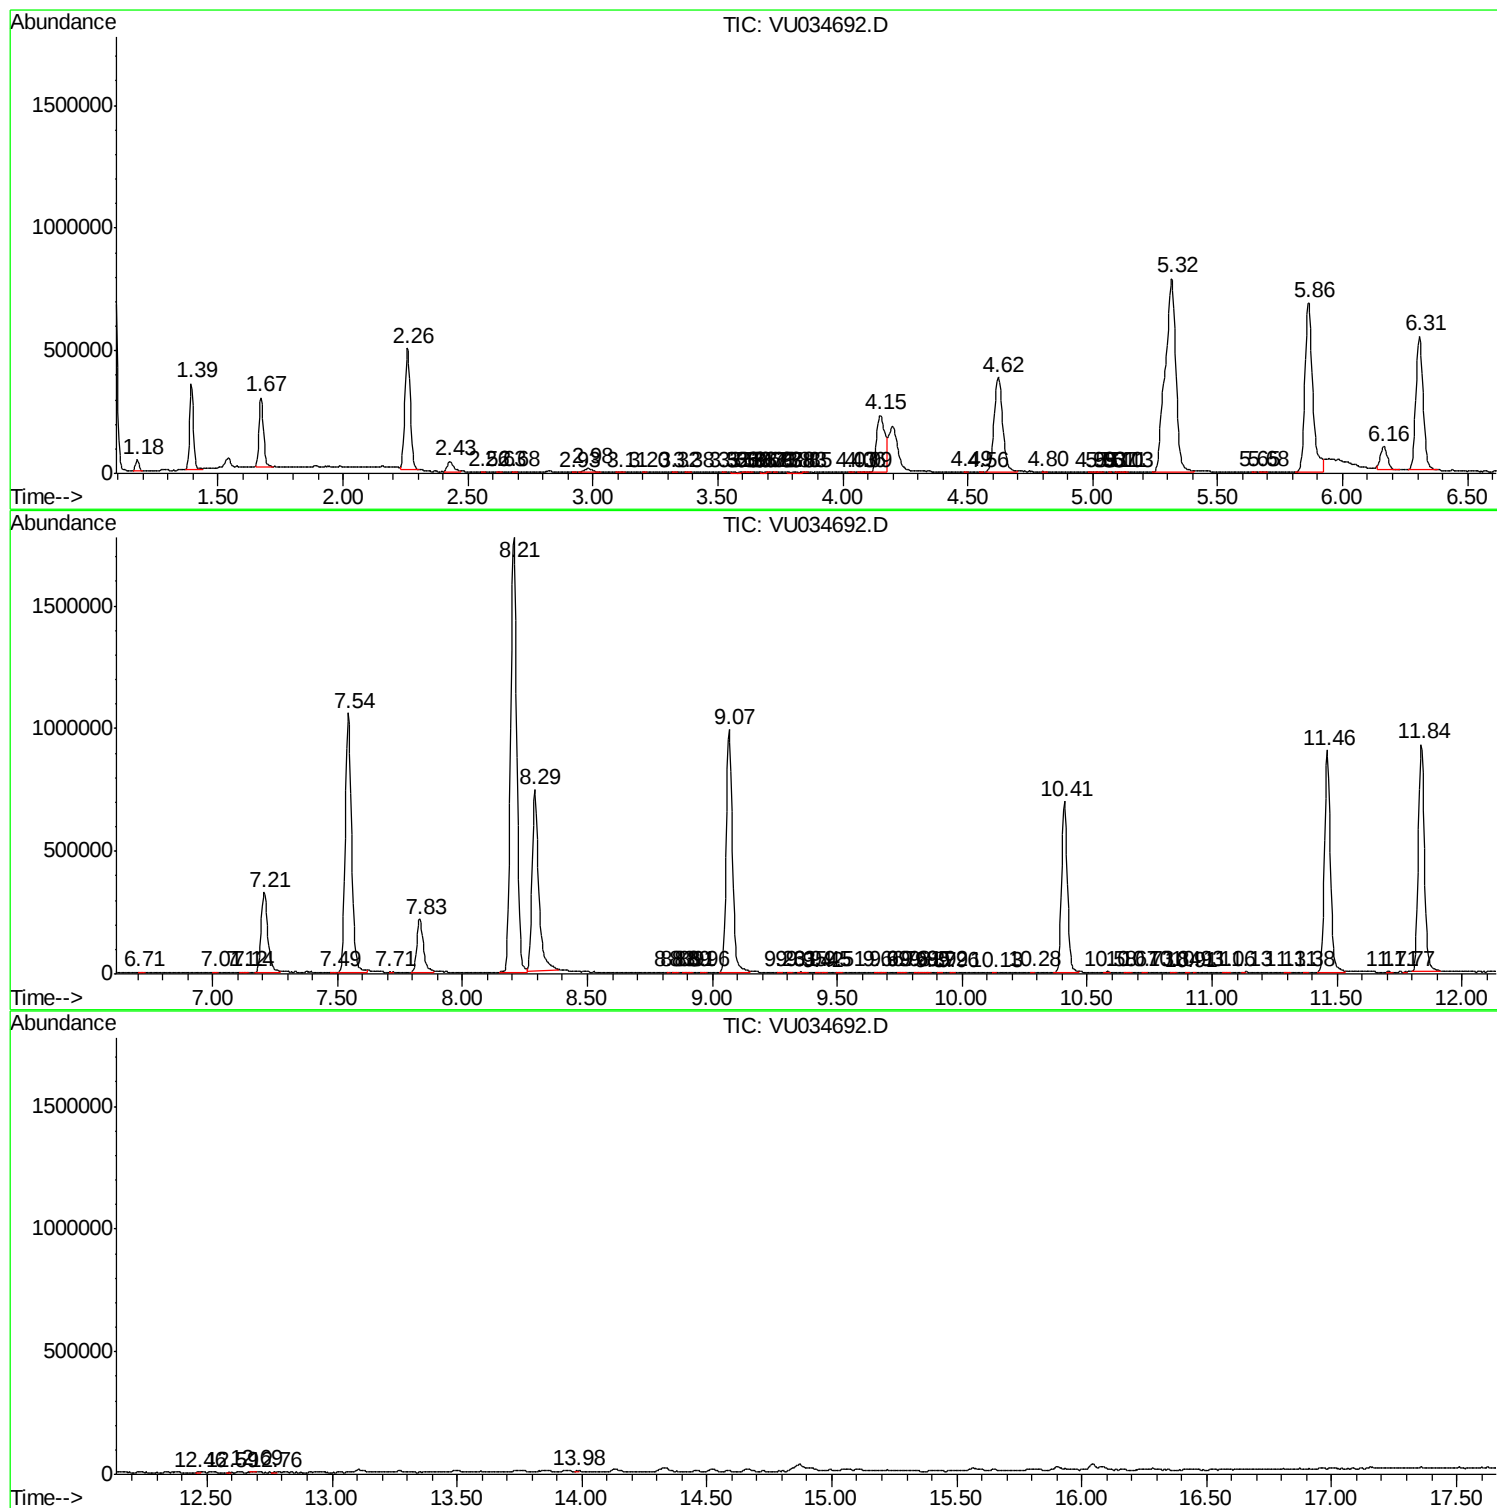

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034692.D
Acq On : 20 Sep 2019 16:31
Operator : JC/SP
Sample : K4948-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDN5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092019\
Data File : VU034692.D
Acq On : 20 Sep 2019 16:31
Operator : JC/SP
Sample : K4948-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEDN5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc